

# Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis

Enzymatic Labeling for Blood,  
Cells, or Tissues (with a High  
Throughput option)

## Protocol

Version 7.4, August 2015

For Research Use Only. Not for use in diagnostic procedures.

Before you begin, view hands-on  
videos of SurePrint procedures at  
<http://www.agilent.com/genomics/protocolvideos>.



Agilent Technologies

# Notices

© Agilent Technologies, Inc. 2009-2015

No part of this manual may be reproduced in any form or by any means (including electronic storage and retrieval or translation into a foreign language) without prior agreement and written consent from Agilent Technologies, Inc. as governed by United States and international copyright laws.

## Manual Part Number

G4410-90010

## Edition

Version 7.4, August 2015

Agilent Technologies, Inc.  
5301 Stevens Creek Blvd.  
Santa Clara, CA 95051 USA

## Technical Support

Technical product support can be obtained by contacting your local Agilent Support Services representative. Agilent's worldwide sales and support center telephone numbers can be obtained at the following web site under **Contact Us**:  
[www.agilent.com/genomics](http://www.agilent.com/genomics)

or send an e-mail to:  
[genomics@agilent.com](mailto:genomics@agilent.com)

## Warranty

**The material contained in this document is provided "as is," and is subject to being changed, without notice, in future editions. Further, to the maximum extent permitted by applicable law, Agilent disclaims all warranties, either express or implied, with regard to this manual and any information contained herein, including but not limited to the implied warranties of merchantability and fitness for a particular purpose. Agilent shall not be liable for errors or for incidental or consequential damages in connection with the furnishing, use, or performance of this document or of any information contained herein. Should Agilent and the user have a separate written agreement with warranty terms covering the material in this document that conflict with these terms, the warranty terms in the separate agreement shall control.**

## Technology Licenses

The hardware and/or software described in this document are furnished under a license and may be used or copied only in accordance with the terms of such license.

## Restricted Rights Legend

U.S. Government Restricted Rights. Software and technical data rights granted to the federal government include only those rights customarily provided to end user customers. Agilent provides this customary commercial license in Software and technical data pursuant to FAR 12.211 (Technical Data) and 12.212 (Computer Software) and, for the Department of Defense, DFARS 252.227-7015 (Technical Data - Commercial Items) and DFARS 227.7202-3 (Rights in Commercial Computer Software or Computer Software Documentation).

## Safety Notices

### CAUTION

A **CAUTION** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in damage to the product or loss of important data. Do not proceed beyond a **CAUTION** notice until the indicated conditions are fully understood and met.

---

### WARNING

A **WARNING** notice denotes a hazard. It calls attention to an operating procedure, practice, or the like that, if not correctly performed or adhered to, could result in personal injury or death. Do not proceed beyond a **WARNING** notice until the indicated conditions are fully understood and met.

---

## In This Guide...

This guide describes the Agilent recommended operational procedures to analyze DNA copy number variations using Agilent 60-mer oligonucleotide microarrays for array-based comparative genomic hybridization (aCGH) analysis. This protocol is specifically developed and optimized to enzymatically label DNA from blood, cells or frozen tissues. For processing FFPE samples, follow the *Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis (ULS Labeling for Blood, Cells, Tissues or FFPE) Protocol* (p/n G4410-90020). FFPE samples are not supported for SurePrint G3 CGH+SNP microarray processing.

### **1 Before You Begin**

This chapter contains information (such as procedural notes, safety information, required reagents and equipment) that you should read and understand before you start an experiment.

### **2 DNA Isolation**

This chapter describes the method to isolate genomic DNA (gDNA) from blood, cells, or frozen tissues.

### **3 Sample Preparation**

This chapter describes the standard method to process gDNA prior to labeling as well as the Whole Genome Amplification method for low input DNA projects.

### **4 Sample Labeling**

This chapter describes the steps to differentially label the gDNA samples with fluorescent-labeled nucleotides.

### **5 Microarray Processing**

This chapter describes the steps to hybridize, wash and scan Agilent CGH and CGH+SNP microarrays and to extract data using the Agilent Feature Extraction Software for use in Agilent CytoGenomics and Genomics Workbench. It also tells you how to get the Agilent Reference Genotype Files (Male and Female)

for use in Agilent CytoGenomics and Agilent Genomic Workbench.

## **6 Troubleshooting**

This chapter contains possible causes for above-threshold DLRSD (Derivative Log Ratio Standard Deviation). A poor DLRSD score reflects high probe-to-probe log ratio noise.

## **7 Reference**

This chapter contains reference information related to the amplification, labeling, hybridization and wash kits, and the protocol.

## **What's new in 7.4**

- Updated list of supported microarrays and reorganized by species.
- Added reference to compatibility matrix for non-Agilent scanners.
- Updated product labeling statement.

## **What's new in 7.3**

- Added note to calibrate hybridization oven on a regular basis for accuracy of the collected data.
- Removed support for obsolete Genomic DNA Enzymatic Labeling Kit.
- Changed denaturation temperature to 98°C for primer annealing during labeling and for preparation for hybridization.
- Changed hybridization temperature to 67°C.

## **What's new in 7.2**

- Agilent Purification Columns replace Amicon Ultra columns.
- Support for new SurePrint G3 Human CGH Bundles.

# Content

<b>1</b>	<b>Before You Begin</b>	<b>9</b>
	Procedural Notes	10
	Safety Notes	11
	Agilent Oligo CGH Microarray Kit Contents	12
	Required Equipment	19
	Required Reagents	22
	Required Hardware and Software	25
<b>2</b>	<b>DNA Isolation</b>	<b>27</b>
	Step 1. gDNA Extraction	30
	Step 2. gDNA Quantitation and Quality Analysis	33
<b>3</b>	<b>Sample Preparation</b>	<b>37</b>
	Direct Method	38
	Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit	40
	Amplification Method	43
	Step 1. Fragmentation	45
	Step 2. Library Preparation	46
	Step 3. Amplification	47
	Step 4. Purification of PCR products	48
	Step 5. Quantitation of Amplified-Purified DNA	49
	Step 6. Preparation of Amplified-Purified DNA before Labeling	49
<b>4</b>	<b>Sample Labeling</b>	<b>51</b>
	Step 1. Fluorescent Labeling of gDNA	52
	Step 2. Purification of Labeled gDNA	56
	To determine yield, and degree of labeling or specific activity	61

<b>5</b>	<b>Microarray Processing</b>	<b>63</b>
	Hybridization	64
	Step 1. Prepare the 10× Blocking Agent	64
	Step 2. Prepare labeled gDNA for hybridization	65
	Step 3. Prepare the hybridization assembly	68
	Step 4. Hybridize	69
	Microarray Wash	70
	Step 1. Prewarm Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 (overnight)	71
	Step 2. Wash with Milli-Q ultrapure water	71
	Step 3. Clean with Acetonitrile (Wash Procedure B Only)	72
	Step 4. Prewarm Stabilization and Drying Solution (Wash Procedure B Only)	72
	Step 5. Wash microarrays	74
	Step 6. Put slides in a slide holder	79
	Microarray Scanning and Analysis	81
	Step 1. Scan the microarray slides	81
	Step 2. Analyze microarray image	83
	Step 3. Download Agilent Reference Genotype File	87
<b>6</b>	<b>Troubleshooting</b>	<b>89</b>
	If you have a low OD260/230 or OD260/280 value	90
	If you have poor sample quality due to residual RNA	90
	If you get poor sample quality due to degradation	91
	If the estimated concentration is too high or low	92
	If you have low specific activity or degree of labeling not due to poor sample quality	93
	If you have low yield not due to poor sample quality	93
	If you have post-labeling signal loss	94
	If you have high BGNoise values	95
	If you have poor reproducibility	95

<b>7</b>	<b>Reference</b>	<b>97</b>
	Reagent Kit Components	98
	Microarray Handling Tips	101
	Agilent Microarray Layout and Orientation	102
	Array/Sample tracking on microarray slides	105







# 1 Before You Begin

Procedural Notes	10
Safety Notes	11
Agilent Oligo CGH Microarray Kit Contents	12
Required Equipment	19
Required Reagents	22
Required Hardware and Software	25

Make sure that you read and understand the information in this chapter and have the necessary equipment and reagents listed before you start an experiment.



## Procedural Notes

- Follow the procedure described in this document to isolate gDNA from blood, cells, or frozen tissues, to increase the likelihood of a successful experiment. For processing FFPE samples, refer to the *Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis (ULS Labeling for Blood, Cells, Tissues, or FFPE) Protocol* (p/n G4410-90020). FFPE samples are not supported when you process SurePrint G3 CGH+SNP microarrays.
- If the DNA isolation procedure described in this document cannot be followed, make sure that the DNA is free of RNA and protein contamination.
- To prevent contamination of reagents by nucleases, always wear powder-free laboratory gloves, and use dedicated solutions and pipettors with nuclease-free aerosol-resistant tips.
- Maintain a clean work area.
- Do not mix stock solutions and reactions containing gDNA or enzymes on a vortex mixer. Instead, mix the solutions and reactions by gently tapping the tube with your finger.
- Avoid repeated freeze-thaw cycles of solutions containing gDNA or enzymes.
- When preparing frozen reagent stock solutions for use:
  - 1 Thaw the aliquot as quickly as possible without heating above room temperature.
  - 2 Mix briefly on a vortex mixer, and then spin in a microcentrifuge for 5 to 10 seconds to drive the contents off the walls and lid.
  - 3 Store on ice or in a cold block until use.
- In general, follow Biosafety Level 1 (BL1) safety rules.

## Safety Notes

### CAUTION

Wear appropriate personal protective equipment (PPE) when working in the laboratory.

---

### WARNING

- **Cyanine reagents are considered hazardous by the OSHA Hazard Communication Standard (29 CFR 1910.1200). Contains material that causes damage to the following organs: kidneys, liver, cardiovascular system, respiratory tract, skin, eye lens or cornea, stomach. May be harmful if swallowed. Avoid contact with eyes, skin and clothing.**
  - **2× HI-RPM Hybridization Buffer is considered hazardous by the OSHA Hazard Communication Standard (29 CFR 1910.1200). Contains material that causes damage to the following organs: skin, central nervous system. May be harmful if swallowed. Avoid contact with eyes, skin and clothing.**
  - **Triton is harmful if swallowed. Risk of serious damage to eyes. Wear suitable PPE. Triton is a component of the Agilent 2× HI-RPM Hybridization Buffer.**
  - **Stabilization and Drying Solution is considered hazardous by the OSHA Hazard Communication Standard (29 CFR 1910.1200). Flammable liquid and vapor. Keep away from heat, sparks and flame. Keep container closed. Use only with adequate ventilation. This solution contains material which causes damage to the following organs: kidneys, liver, cardiovascular system, upper respiratory tract, skin, central nervous system (CNS), eye, lens or cornea.**
-

## Agilent Oligo CGH Microarray Kit Contents

Store microarray kit at room temperature. After the microarray foil pouch is opened, store the microarray slides at room temperature (in the dark) under a vacuum desiccator or N<sub>2</sub> purge box. Do not store microarray slides in open air after breaking foil.

### SurePrint G3 CGH Bundle

- 1-inch × 3-inch microarray slides in quantities of:
  - 50 for 1-pack
  - 25 for 2-pack
  - 12 for 4-pack
  - 6 for 8-pack
- Sufficient reagents and consumables to process 50 (1-pack and 2-pack bundle) or 48 (4-pack and 8-pack bundle) samples:
  - SureTag Complete DNA Labeling Kit
  - Oligo aCGH/ChIP-on-chip Hybridization Kit
  - Hybridization gasket slides
  - Human Cot-1 DNA
  - Oligo aCGH/ChIP-on-chip Wash Buffer 1 and Oligo aCGH/ChIP-on-chip Wash Buffer 2
  - Agilent CytoGenomics Software License

**Table 1** SurePrint G3 CGH and CGH+SNP Bundles

Part Number	Description
G5920A, Option 1	SurePrint G3 Human CGH Bundle, 1×1M
G5921A, Option 1	SurePrint G3 Human CGH Bundle, 2×400K
G5921A, Option 2	SurePrint G3 CGH+SNP Bundle, 2×400K
G5922A, Option 1	SurePrint G3 Human CGH Bundle, 4×180K
G5922A, Option 2	SurePrint G3 ISCA CGH+SNP Bundle, 4×180K
G5923A, Option 1	SurePrint G3 Human CGH Bundle, 8×60K

### Catalog SurePrint HD and G3 CGH Microarray Kits

- Five 1-inch × 3-inch, 1-pack and 2-pack microarray slides
- Three 1-inch × 3-inch, 4-pack and 8-pack microarray slides

Design files can be downloaded from  
<http://www.agilent.com/genomics/suredesign>.

See the tables that follow for available designs. For more information on CGH designs, go to <http://www.genomics.agilent.com>. Under **Products**, click **CGH & CGH+SNP Microarrays**.

**Table 2** Catalog SurePrint CGH+SNP Microarray Kits - Human

Part Number	Description
G4842A*	SurePrint G3 Human CGH+SNP Microarray Kit 2×400K
G4890A*	SurePrint G3 Human ISCA CGH+SNP Microarray Kit 4×180K
G4869A*	SurePrint G3 Human Cancer CGH+SNP Microarray Kit 4×180K

\* These arrays can only be processed using the enzymatic labeling protocol.

**1 Before You Begin**  
**Agilent Oligo CGH Microarray Kit Contents**

**Table 3** Catalog CGH Microarray Kits - Human

<b>Part Number</b>	<b>Description</b>
G4447A	SurePrint G3 Human CGH Microarray Kit 1×1M (5 slides)
G4824A-021529	SurePrint G3 Human CGH Microarray Slide 1×1M
G4448A	SurePrint G3 Human CGH Microarray Kit 2×400K (5 slides)
G4825A-021850	SurePrint G3 Human CGH Microarray Slide 2×400K
G4449A	SurePrint G3 Human CGH Microarray Kit 4×180K (5 slides)
G4826A-022060	SurePrint G3 Human CGH Microarray Slide 4×180K
G4450A	SurePrint G3 Human CGH Microarray Kit 8×60K (5 slides)
G4827A-021924	SurePrint G3 Human CGH Microarray Slide 8×60K
G4423B-016266	SurePrint G3 Human CGH 244A Supplemental Slide 1×244K
G5955A	SurePrint G3 Human CGH ISCA v2 Microarray Kit 8×60K (3 slides)
G4411B	Human Genome CGH 244A Microarray Kit 1×244K (5 slides)
G4423B-014693	Human Genome CGH 244A Microarray Slide 1×244K
G4412A	Human Genome CGH 105A Microarray Kit 2×105K
G4425B-014698	Human Genome CGH 105A Microarray Slide 2×105K
G4413A	Human Genome CGH Microarray Kit 4×44K (3 slides)
G4426B-014950	Human Genome CGH Microarray Slide 4×44K

**Table 4** Catalog CNV Microarray Kits - Human

Part Number	Description
G4506A	SurePrint G3 Human CNV Microarray Kit 1×1M (5 slides)
G4824A-023642	SurePrint G3 Human CNV Microarray Slide 1×1M
G4507A	SurePrint G3 Human CNV Microarray Kit 2×400K (5 slides)
G4825A-021365	SurePrint G3 Human CNV Microarray Slide 2×400K
G4423B-018897	SurePrint G3 Human CNV Microarray Slide, Slide 1 of 2, 1×244K
G4423B-018898	SurePrint G3 Human CNV Microarray Slide, Slide 2 of 2, 1×244K
G4417A	Human CNV Association Microarray Kit 2×105K (5 slides)
G4425B-022837	Human CNV Association Microarray Slide 2×105K

**Table 5** Catalog CGH Microarrays- Mouse

Part Number	Description
G4838A	SurePrint G3 Mouse CGH Microarray Kit 1×1M (5 slides)
G4824A-027414	SurePrint G3 Mouse CGH Microarray Slide 1×1M
G4839A	SurePrint G3 Mouse CGH Microarray Kit 4×180K (3 slides)
G4826A-027411	SurePrint G3 Mouse CGH Microarray Kit 4×180K
G4415A	Mouse Genome CGH Microarray Kit 1×244K (5 slides)
G4423B-014695	Mouse Genome CGH Microarray Slide 1×244K
G4416A	Mouse Genome CGH Microarray Kit 2×105K (5 slides)
G4425B-014699	Mouse Genome CGH Microarray Slide 2×105K

## 1 Before You Begin

### Agilent Oligo CGH Microarray Kit Contents

**Table 6** Catalog CGH Microarrays - Rat

Part Number	Description
G4840A	SurePrint G3 Rat CGH Microarray Kit 1×1M (5 slides)
G4824A-027065	SurePrint G3 Rat CGH Microarray Slide 1×1M
G4841A	SurePrint G3 Rat CGH Microarray Kit 4×180K (3 slides)
G4826A-027064	SurePrint G3 Rat CGH Microarray Slide 4×180K
G4435A	Rat Genome CGH Microarray Kit 1×244K (5 slides)
G4423B-015223	Rat Genome CGH Microarray Slide 1×244K
G4436A	Rat Genome CGH Microarray Kit 2×105K (5 slides)
G4425B-015235	Rat Genome CGH Microarray Slide 2×105K

**Table 7** Catalog CGH Microarrays - Model Organism/Non-Human

Part Number	Description
G4826A-024419	SurePrint G3 Rhesus Macaque CGH Microarray Kit 4×180K (5 slides)
G4826A-024422	SurePrint G3 Chimpanzee CGH Microarray Kit 4×180K (5 slides)
G4826A-025242	SurePrint G3 Bovine CGH Microarray Kit 4×180K (5 slides)
G4826A-025522	SurePrint G3 Canine CGH Microarray Kit 4×180K (5 slides)
G4826A-025843	SurePrint G3 Rice CGH Microarray Slide 4×180K
G4423B-019553	Chicken Genome CGH Microarray, 1×244K

### Unrestricted SurePrint HD and G3 CGH Microarrays

- One, two, four or eight microarrays printed on each 1-inch × 3-inch glass slide
- Number of microarray slides vary per kit and per order

Design files can be downloaded from  
<http://www.agilent.com/genomics/suredesign>.

See the tables that follow for available designs.



**Table 8** Unrestricted CGH Microarrays - Human

Part Number	Description
G4826A, AMADID 031748	Unrestricted SurePrint G3 CGH ISCA v2 Microarray, 4×180K
G4827A, AMADID 031746	Unrestricted SurePrint G3 CGH ISCA v2 Microarray, 8×60K
G4425B, AMADID 031750	Unrestricted HD CGH ISCA v2 Microarray, 2×105K
G4426B, AMADID 031747	Unrestricted HD CGH ISCA v2 Microarray, 4×44K

### Custom SurePrint HD and G3 Microarrays

- One, two, four or eight microarray(s) printed on each 1-inch × 3-inch glass slide
- Number of microarrays varies per kit and per order

See the tables that follow for available formats.

**Table 9** Custom SurePrint G3 CGH and CGH+SNP Microarrays

Part Number	Description
G4882A*	SurePrint G3 Custom CGH+SNP Microarray, 1×1M
G4883A*	SurePrint G3 Custom CGH+SNP Microarray, 2×400K
G4884A*	SurePrint G3 Custom CGH+SNP Microarray, 4×180K
G4885A*	SurePrint G3 Custom CGH+SNP Microarray, 8×60K
G4123A	SurePrint G3 Custom CGH Microarray, 1×1M
G4124A	SurePrint G3 Custom CGH Microarray, 2×400K
G4125A	SurePrint G3 Custom CGH Microarray, 4×180K
G4126A	SurePrint G3 Custom CGH Microarray, 8×60K

\* These arrays can only be processed using the enzymatic labeling protocol.

## 1 Before You Begin

### Agilent Oligo CGH Microarray Kit Contents

**Table 10** Custom SurePrint HD CGH Microarrays

Part Number	Description
G4423A	Custom HD-CGH Microarray, 1×244K
G4425A	Custom HD-CGH Microarray, 2×105K
G4426A	Custom HD-CGH Microarray, 4×44K
G4427A	Custom HD-CGH Microarray, 8×15K

## Required Equipment

**Table 11** Required equipment

Description	Vendor and part number
200 µL Thin-Wall Tube	Agilent p/n 410091 or equivalent
Agilent Microarray Scanner Bundle for 1×244K, 2×105K, 4×44K or 8×15K, <i>or</i> for 1×1M, 2×400K, 4×180K or 8×60K	Agilent p/n G4900DA, G2565CA or G2565BA Agilent p/n G4900DA or G2565CA
Hybridization Chamber, stainless	Agilent p/n G2534A
Hybridization gasket slides, 5-pack (20 and 100 packaging sizes are available)* for 1-pack microarrays <i>or</i> for 2-pack microarrays <i>or</i> for 4-pack microarrays <i>or</i> for 8-pack microarrays	Agilent p/n G2534-60003 Agilent p/n G2534-60002 Agilent p/n G2534-60011 Agilent p/n G2534-60014
Hybridization oven; temperature set at 67°C	Agilent p/n G2545A
Hybridization oven rotator for Agilent Microarray Hybridization Chambers	Agilent p/n G2530-60029
Ozone-barrier slide covers (box of 20) <sup>†</sup>	Agilent p/n G2505-60550
Thermal cycler with heated lid	Agilent p/n G8800A or equivalent
UV-Transilluminator with SYBR photographic filter	Alpha Innotech p/n Alphamager 2000 or equivalent
1.5 mL RNase-free Microfuge Tube (sustainable at 98°C)	Ambion p/n AM12400 or equivalent
Magnetic stir plate (×1 or ×3) <sup>‡‡</sup>	Corning p/n 6795-410 or equivalent
Magnetic stir plate with heating element	Corning p/n 6795-420 or equivalent
Microcentrifuge	Eppendorf p/n 5430 or equivalent
E-Gel Opener <sup>†</sup>	Life Technologies p/n G5300-01
E-Gel PowerBase v.4 <sup>†</sup>	Life Technologies p/n G6200-04
Qubit Fluorometer <sup>**</sup>	Life Technologies p/n Q32857
Thin wall, clear 0.5 mL PCR tubes <sup>**</sup>	Life Technologies p/n Q32856 <i>or</i> VWR p/n 10011-830

## 1 Before You Begin

### Required Equipment

**Table 11** Required equipment (continued)

Description	Vendor and part number
Sterile storage bottle	Nalgene 455-1000 or equivalent
UV-VIS spectrophotometer	NanoDrop 8000 or 2000, or equivalent
P10, P20, P200 and P1000 pipettes	Pipetman P10, P20, P200, P1000 or equivalent
1.5 L glass dish	Pyrex p/n 213-R or equivalent
Vacuum Concentrator ††	Thermo Scientific Savant SpeedVac p/n DNA120-115 or equivalent
Magnetic stir bar, 7.9 × 38.1 mm (×2 or ×4) ††	VWR p/n 58948-150 or equivalent
250 mL capacity slide-staining dish, with slide rack (×3 or ×5) ††	Wheaton p/n 900200 <i>or</i> Thermo Shandon p/n 121
Circulating water baths or heat blocks. For DNA extraction, set to 56°C. For restriction digestion and/or labeling, set to 37°C, 65°C and 98°C.	
Ice bucket	
Clean forceps	
Powder-free gloves	
Sterile, nuclease-free aerosol barrier pipette tips	
Timer	
Vacuum desiccator or N <sub>2</sub> purge box for slide storage	
Vortex mixer	

\* Included in the [SurePrint G3 CGH Bundle](#).

† Optional. Recommended when processing arrays with a G2565CA or G2565BA scanner in environments in which ozone levels are 5 ppb or higher.

‡ For use with Life Technologies E-gels.

\*\* Optional.

†† Optional. Depends on microarray format and processing protocol used.

‡‡ The number varies depending on if wash procedure A or B is selected.

**Table 12** Optional. Recommended when using the high throughput or amplification method for sample preparation.

Description	Vendor and part number
Thermal cycler with heated lid	Agilent p/n G8800A or equivalent
96-well PCR plate	Agilent p/n 401334 or equivalent
Centrifuge (for 96-well plate)	Eppendorf p/n 5810 or equivalent
Heat Sealer	Eppendorf p/n 951023078
Peel-it-lite Foil (removable)	Eppendorf p/n 951023205

**Table 13** Optional. Recommended when using high-throughput method on 2-pack microarrays.

Description	Vendor and part number
Tall Chimney PCR plate	ABgene p/n AB-1184

**Table 14** Optional equipment for DNA extraction from tissue.

Description	Vendor and part number
Thermal shaker	Eppendorf Thermomixer p/n 022670000 or equivalent

## Required Reagents

**Table 15** Required reagents for gDNA isolation

Description	Vendor and part number
Phosphate Buffered Saline pH 7.4 (PBS)	Amresco p/n E504-500ML
Clear E-Gel (1.2% agarose, no stain), 18-pack	Life Technologies p/n G5518-01
SYBR Gold Nucleic Acid Gel Stain	Life Technologies p/n S11494
SYBR photographic filter	Life Technologies p/n S7569
TrackIt 1 Kb DNA Ladder	Life Technologies p/n 10488-072
DNase/RNase-free distilled water	Life Technologies p/n 10977-015
Qubit dsDNA BR Assay Kit, for use with the Qubit fluorometer (100 assays)*	Life Technologies p/n Q32850
RNase A (100 mg/mL)	Qiagen p/n 19101
DNeasy Blood & Tissue Kit	Qiagen p/n 69504
Proteinase K (>600 mAU/mL, solution)	Qiagen p/n 19131
Ethanol (95% to 100% molecular biology grade)	Sigma-Aldrich p/n E7023-6×500ML

\* Optional.

**Table 16** Required reagents for enzymatic sample prep and labeling with the SureTag Complete DNA Labeling Kit (for Human Samples)

Description	Vendor and part number
SureTag Complete DNA Labeling Kit <sup>††</sup>	Agilent p/n 5190-4240
Purification Columns <sup>‡</sup> (50 units)	Agilent p/n 5190-3391
AutoScreen A, 96-well plates <sup>**</sup>	GE Healthcare p/n 25-9005-98
1×TE (pH 8.0), Molecular grade	Promega p/n V6231
GenElute PCR Clean-Up Kit <sup>††</sup>	Sigma-Aldrich p/n NA1020
GenomePlex Complete Whole Genome Amplification Kit <sup>††</sup>	Sigma-Aldrich p/n WGA2

\* Kit content is listed in “Reagent Kit Components” on page 98.

† Included in the SurePrint G3 CGH Bundle.

‡ Included in the SureTag Complete DNA Labeling Kit. Order additional columns when processing more than 25 8-pack microarrays.

\*\* Optional. Recommended if using the high-throughput protocol.

†† Optional. Recommended if using the Amplification Method for sample preparation.

## 1 Before You Begin

### Required Reagents

**Table 17** Required reagents for enzymatic sample prep and labeling with the [SureTag DNA Labeling Kit](#) (or when Human reference DNA is provided separately)

Description	Vendor and part number
SureTag DNA Labeling Kit <sup>*</sup>	Agilent p/n 5190-3400
Purification Column <sup>†</sup> (50 units)	Agilent p/n 5190-3391
AutoScreen A, 96-well plate <sup>‡</sup>	GE Healthcare p/n 25-9005-98
For possible use as a reference sample:	
<ul style="list-style-type: none"> <li>• Human Genomic DNA <i>or</i></li> <li>• Mouse Genomic DNA <i>or</i></li> <li>• Rat Genomic DNA</li> </ul>	<ul style="list-style-type: none"> <li>• For CGH microarrays: Promega p/n G1521 (female) or p/n G1471 (male)</li> <li>• For CGH+SNP microarrays: Coriell p/n NA18507, NA18517, NA12891, NA12878, or NA18579</li> <li>• Jackson Labs p/n 000664 (female and male)</li> <li>• Harlan Sprague Dawley (custom)</li> </ul>
1×TE (pH 8.0), Molecular grade	Promega p/n V6231
GenElute PCR Clean-Up Kit <sup>**</sup>	Sigma-Aldrich p/n NA1020
GenomePlex Complete Whole Genome Amplification Kit <sup>**</sup>	Sigma-Aldrich p/n WGA2

<sup>\*</sup> Kit content is listed in “[Reagent Kit Components](#)” on page 98.

<sup>†</sup> Included in the [SureTag DNA Labeling Kit](#). Order additional columns when processing more than 25 8-pack microarrays.

<sup>‡</sup> Optional. Recommended if using the high-throughput protocol.

<sup>\*\*</sup> Optional. Recommended if using the Amplification Method for sample preparation.



**Table 18** Required reagents for hybridization and wash

Description	Vendor and part number
Oligo aCGH/ChIP-on-chip Wash Buffer Kit <i>or</i>	Agilent p/n 5188-5226
Oligo aCGH/ChIP-on-chip Wash Buffer 1 <i>and</i>	Agilent p/n 5188-5221
Oligo aCGH/ChIP-on-chip Wash Buffer 2 <sup>*</sup>	Agilent p/n 5188-5222
Stabilization and Drying Solution <sup>†</sup>	Agilent p/n 5185-5979
Oligo aCGH/ChIP-on-chip Hybridization Kit <sup>*</sup>	Agilent p/n 5188-5220 (25) or p/n 5188-5380 (100)
Cot-1 DNA (1.0 mg/mL)	
• Human Cot-1 DNA <sup>*</sup> <i>or</i>	Agilent p/n 5190-3393
• Mouse Cot-1 DNA <i>or</i>	Life Technologies p/n 18440-016
• Rat Hybloc	Applied Genetics p/n RHB
DNase/RNase-free distilled water	Life Technologies p/n 10977-015
Milli-Q ultrapure water	Millipore
Acetonitrile <sup>†</sup>	Sigma-Aldrich p/n 271004-1L


<sup>\*</sup> Included in the [SurePrint G3 CGH Bundle](#).

<sup>†</sup> Optional components recommended if wash procedure B is selected.

## Required Hardware and Software

- Refer to the Agilent Scanner manual and Agilent CytoGenomics or Feature Extraction manuals for minimum memory requirements and other specifications. Go to <http://www.genomics.agilent.com>.

**This page intentionally left blank.**

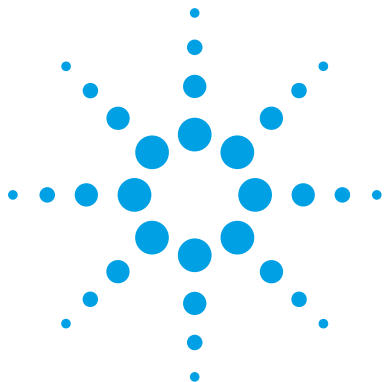

## 2 DNA Isolation

Step 1. gDNA Extraction 30

Step 2. gDNA Quantitation and Quality Analysis 33

### NOTE

Agilent cannot guarantee microarray performance and does not provide technical support to those who use non-Agilent protocols in processing Agilent microarrays.

The Agilent array-based Comparative Genomic Hybridization (aCGH) application uses a “two-color” process to measure DNA copy number changes (CNC), and copy-neutral Loss of Heterozygosity or Uniparental Disomy if CGH+SNP microarrays are used, in an experimental sample relative to a reference sample. The type of sample used as a reference is a matter of experimental choice; however, many experimenters use normal commercial gDNA as a reference sample, such as the [Human Reference DNA \(Male and Female\)](#) that is included in the [SureTag Complete DNA Labeling Kit](#).

This chapter describes the Agilent recommended procedure for isolating gDNA from blood, cells, or frozen tissues using the [DNeasy Blood & Tissue Kit](#).

For processing FFPE samples, follow the *Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis (ULS Labeling for Blood, Cells, Tissues, or FFPE) Protocol* (p/n G4410-90020). FFPE samples are not supported when you process SurePrint G3 CGH+SNP microarrays.


### CGH+SNP Microarrays

When you process SurePrint G3 CGH+SNP microarrays, the reference needs to be DNA isolated from a single genotyped individual. You can use one of the following DNA samples as reference:



- 1** Human Reference DNA Male or Female, components of the [SureTag Complete DNA Labeling Kit](#).
- 2** One of five supported HapMap samples: NA18507 (Yoruban Male), NA18517 (Yoruban Female), NA12891 (European Male), NA12878 (European Female), or NA18579 (Chinese Female). The HapMap samples can be ordered from the Coriell Institute for Medical Research.
- 3** You can genotype your own reference DNA isolated from a single individual by hybridizing it against all 5 supported HapMap samples on the Agilent CGH+SNP microarrays. This experiment only needs to be done once.

The input amount of DNA for the experimental sample labeling reaction must be the same as for the reference sample labeling reaction. Inaccurate DNA quantitation can lead to different DNA inputs into the experimental and reference labeling reactions, which increases assay noise (DLRSD). Different DNA isolation methods can also create quantitation artifacts. To minimize assay noise, Agilent recommends to use a fluorometric method (such as Qubit) highly selective for double-stranded DNA. A Nanodrop spectrophotometer can be used to assess gDNA purity. There is no need to re-determine the concentration of the Agilent Human Reference DNA Male and Female, its concentration is 200 ng/ $\mu$ L as measured by both spectrophotometer and fluorometer.

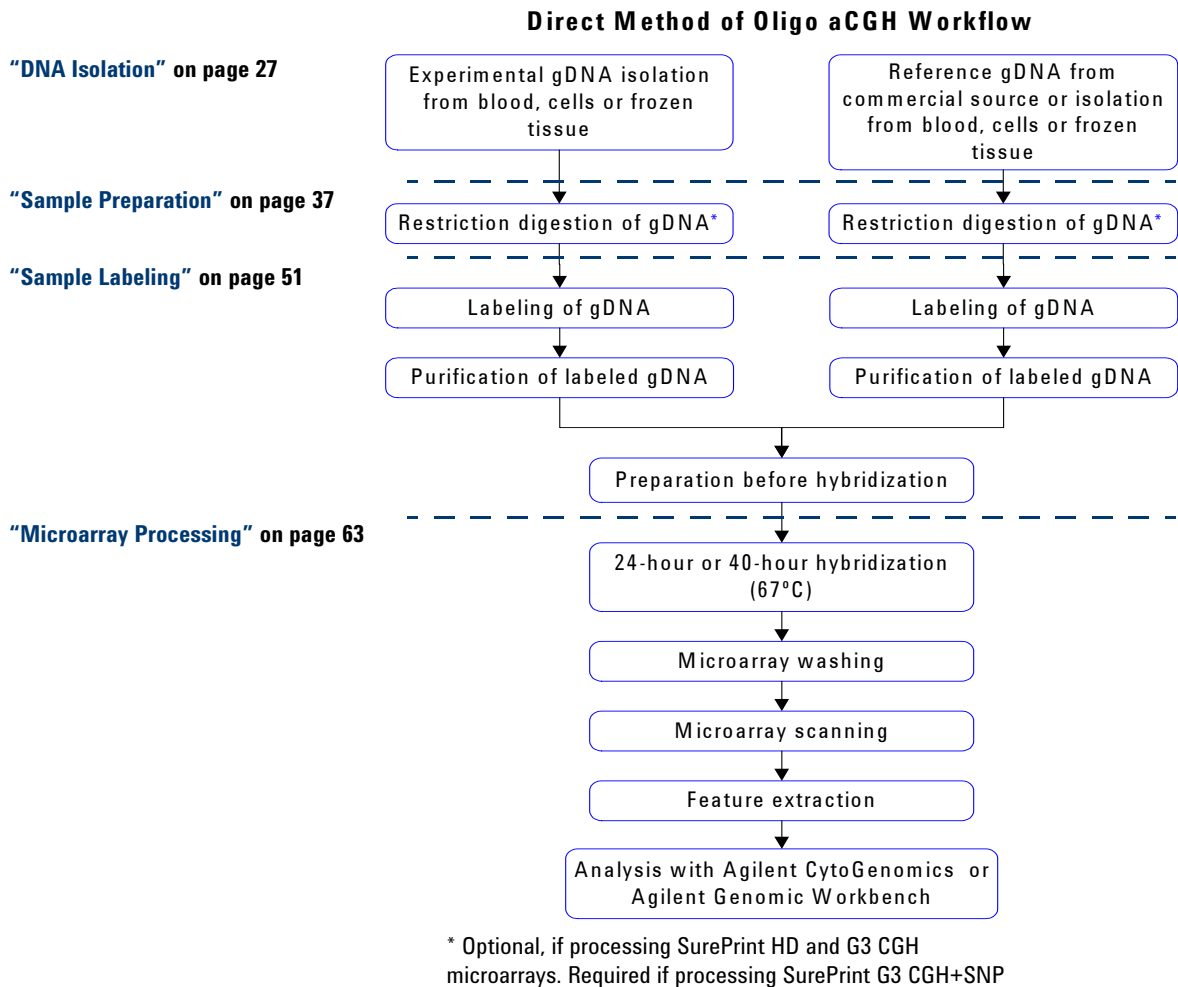

**Figure 1** Direct workflow for sample preparation and microarray processing. Minimum of 0.5  $\mu\text{g}$  (for 1-pack, 2-pack or 4-pack microarrays) or 0.2  $\mu\text{g}$  (for 8-pack microarrays) starting gDNA per sample is required.

## Step 1. gDNA Extraction

Use reagents from the DNeasy Blood & Tissue Kit.

- 1** Equilibrate a thermomixer and heat block or water bath to 56°C.
- 2** For blood with nonnucleated erythrocytes (mammals):
  - a** Put 20 µL of Proteinase K into the bottom of a 1.5 mL RNase-free Microfuge Tube.
  - b** Add 50 to 100 µL of anticoagulated blood.
  - c** Add enough Phosphate Buffered Saline pH 7.4 (PBS) to make a total volume of 220 µL.
  - d** Go to step 7.
- 3** For blood with nucleated erythrocytes (such as chicken):
  - a** Put 20 µL of Proteinase K into the bottom of a 1.5 mL RNase-free Microfuge Tube.
  - b** Add 5 to 10 µL of anticoagulant blood.
  - c** Add enough Phosphate Buffered Saline pH 7.4 (PBS) to make a total volume of 220 µL.
  - d** Go to step 7.
- 4** For cells:
  - a** Spin a maximum of  $5 \times 10^6$  cells in a centrifuge for 5 minutes at  $300 \times g$ . Resuspend the pellet in 200 µL of Phosphate Buffered Saline pH 7.4 (PBS).
  - b** Add 20 µL of Proteinase K.
  - c** Go to step 7.
- 5** For frozen tissue:
  - a** Cut up to 25 mg frozen tissue (up to 10 mg for spleen tissue) into small pieces and put into a 1.5 mL RNase-free Microfuge Tube.
  - b** Add 180 µL of Buffer ATL.
  - c** Add 20 µL of Proteinase K.
  - d** Mix well on a vortex mixer.
  - e** Incubate in a thermomixer at 56°C shaking at 450 rpm until the tissue is completely lysed.

Lysis time varies depending on the type of tissue processed. Usually lysis is complete in 1 to 3 hours. If it is more convenient, samples can be lysed overnight.

- f** Let the sample cool to room temperature and spin in a microcentrifuge for 30 seconds at  $6,000 \times g$  to drive the contents off the walls and lid.
  - g** Go to step 7.
- 6** For further purification of extracted DNA:
    - a** Take a maximum 25  $\mu\text{g}$  of DNA.
    - b** Add enough Phosphate Buffered Saline pH 7.4 (PBS) to make a total volume of 220  $\mu\text{L}$ .
    - c** Add 20  $\mu\text{L}$  of Proteinase K.
  - 7** Add 4  $\mu\text{L}$  of RNase A (100 mg/mL), mix on a vortex mixer, and incubate for 2 minutes at room temperature. Spin in a microcentrifuge for 30 seconds at  $6,000 \times g$  to drive the contents off the walls and lid.
  - 8** Add 200  $\mu\text{L}$  of Buffer AL to each sample, mix thoroughly on a vortex mixer, and incubate at  $56^\circ\text{C}$  for 10 minutes in a heat block or water bath. Spin in a microcentrifuge for 30 seconds at  $6,000 \times g$  to drive the contents off the walls and lid.
  - 9** Add 200  $\mu\text{L}$  of 100% Ethanol to each sample, and mix thoroughly on a vortex mixer. Spin in a microcentrifuge for 30 seconds at  $6,000 \times g$  to drive the contents off the walls and lid.
  - 10** Transfer the sample mixture onto a DNeasy Mini Spin Column in a 2 mL Collection Tube. Spin in a centrifuge at  $6,000 \times g$  for 1 minute. Discard the flow-through and collection tube. Put the DNeasy Mini Spin Column in a new 2 mL Collection Tube.
  - 11** Before using for the first time, prepare Buffer AW1 by adding 100% Ethanol to the Buffer AW1 bottle (see bottle label for volume). Mark the appropriate check box to indicate that ethanol was added to the bottle.
  - 12** Add 500  $\mu\text{L}$  Buffer AW1 onto the column, and spin in a microcentrifuge for 1 minute at  $6,000 \times g$ . Discard the flow-through and collection tube. Put the DNeasy Mini Spin Column in a new 2 mL Collection Tube.
  - 13** Before using for the first time, prepare Buffer AW2 by adding 100% Ethanol to the Buffer AW2 bottle (see bottle label for volume). Mark the appropriate check box to indicate that ethanol was added to the bottle.

## 2 DNA Isolation

### Step 1. gDNA Extraction

- 14** Add 500  $\mu\text{L}$  of **Buffer AW2** onto the column, and spin in a centrifuge for 3 minutes at  $20,000 \times g$  to dry the DNeasy membrane. Discard the flow-through and collection tube.
- 15** Put the **DNeasy Mini Spin Column** in a clean **1.5 mL RNase-free Microfuge Tube**, and pipette 200  $\mu\text{L}$  of **Buffer AE** directly onto the center of the DNeasy column membrane.
- 16** Incubate at room temperature for 1 minute, and then spin in a microcentrifuge for 1 minute at  $6,000 \times g$  to elute the DNA.
- 17** Repeat elution with **Buffer AE** once as described in **step 15** and **step 16**. Combine the duplicate samples in one microcentrifuge tube for a final volume of 400  $\mu\text{L}$ .



## Step 2. gDNA Quantitation and Quality Analysis

Accurate assessment of gDNA quantity and quality are crucial to the success of an Agilent Oligo aCGH experiment. High quality gDNA should be free of contaminants such as carbohydrates, proteins, and traces of organic solvents, and should also be intact with minimal degradation.

See “FFPE Tissues” in the *Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis (ULS Labeling for Blood, Cells, Tissues or FFPE) Protocol* (p/n G4410-90020) for details on how to isolate gDNA from FFPE tissues. FFPE samples are not supported when you process SurePrint G3 CGH+SNP microarrays.

Use Quant-iT dsDNA Broad-Range Assay Kit to measure the concentration of double-strand DNA by fluorometry. Use the NanoDrop ND-1000 UV-VIS Spectrophotometer (or equivalent) to assess gDNA concentration and purity. Use agarose gel electrophoresis to assess gDNA intactness and the average molecular weight for each sample.

### NOTE

Agilent recommends the use of a fluorometric quantitation method for the highest quality data.

### Fluorometry

Use the [Qubit dsDNA BR Assay Kit](#) at room temperature (22°C to 28°C). Temperature fluctuations can affect the accuracy of the assay.

- 1 Set up [Thin wall, clear 0.5 mL PCR tubes](#) for the two standards plus the number of samples you are processing.
- 2 Make a [Qubit working solution](#).

For each standard and sample to be quantified, mix the components in [Table 19](#) together on a vortex mixer for 2 to 3 seconds.

**Table 19** Qubit working solution

Component	Amount
Qubit dsDNA BR reagent	1 µL
Qubit dsDNA BR buffer	199 µL

## 2 DNA Isolation

### Step 2. gDNA Quantitation and Quality Analysis

- 3 Load 190  $\mu\text{L}$  of Qubit working solution into the two Thin wall, clear 0.5 mL PCR tubes labeled for the standards.
- 4 Load 180 to 199  $\mu\text{L}$  of Qubit working solution into the tubes labeled for your samples.
- 5 Add 10  $\mu\text{L}$  of Qubit dsDNA BR standard #1 or Qubit dsDNA BR standard #2 to the appropriate tube.
- 6 Add 1 to 20  $\mu\text{L}$  of your DNA sample to the appropriate tubes.
- 7 Mix the content of all the tubes on a vortex mixer for 2 to 3 seconds. Be careful not to create bubbles.
- 8 Incubate the tubes at room temperature for 2 minutes.
  - To calibrate the Qubit:
    - a On the home screen of the Qubit 1.0, use the up or down arrow to select **dsDNA Broad Range Assay** as assay type, and then press **GO**. The standard screen is automatically displayed.
    - b Select **Run new calibration**, and then press **GO**.
    - c Insert the tube with the first standard into the Qubit Fluorometer, close the lid and press **GO**. After the reading is done, remove the standard.
    - d Insert the tube with the second standard into the Qubit Fluorometer, close the lid, and press **GO**. After the reading is done remove the standard.

The calibration is complete after the second standard has been read.
  - To measure sample concentration:
    - a After the calibration is complete, insert a sample and press **GO**.
    - b When the measurement is complete (approximately 5 seconds later), make a note of the reading.
    - c The result is displayed on the screen. The number displayed is the concentration of the nucleic acid in the assay tube.
    - d Remove the sample from the instrument, insert the next sample, and press **GO**.
    - e Repeat sample readings until all samples have been read.
    - f Calculate the concentration of your original sample.

The Qubit Fluorometer gives a value for the Qubit dsDNA BR assay in  $\mu\text{g}/\text{mL}$ . This value corresponds to the concentration after your samples were diluted into the assay tube. To calculate the concentration of your sample, use this equation:

$$\text{Sample concentration} = QF \text{ value} \times (200/y)$$

where

*QF value* = the value given by the Qubit Fluorometer

*y* = the volume of sample you added to the assay tube.

### UV-VIS Spectrophotometry


- 1 In the Nanodrop program menu, select **Nucleic Acid Measurement**, and then select **Sample Type** to be **DNA-50**.
- 2 Use 1.5  $\mu\text{L}$  of **Buffer AE** to blank the instrument.
- 3 Use 1.5  $\mu\text{L}$  of each gDNA sample to measure DNA concentration. Record the gDNA concentration ( $\text{ng}/\mu\text{L}$ ) for each sample. Calculate the yield as

$$\text{Yield } (\mu\text{g}) = \frac{\text{DNA Concentration } (\text{ng}/\mu\text{L}) \times \text{Sample Volume } (\mu\text{L})}{1000 \text{ ng}/\mu\text{g}}$$

- 4 Record the  $A_{260}/A_{280}$  and  $A_{260}/A_{230}$  ratios. High-quality gDNA samples have an  $A_{260}/A_{280}$  ratio of 1.8 to 2.0, which indicates the absence of contaminating proteins. Scanning the absorbance from 220-320 nm will show whether contaminants exist that affect absorbance at 260 nm. Check the absorbance scans for a peak at 260 nm and an overall smooth shape as shown in [Figure 2](#). The ideal 260/230 ratio for pure DNA is  $>1.0$ .

## 2 DNA Isolation


### Step 2. gDNA Quantitation and Quality Analysis

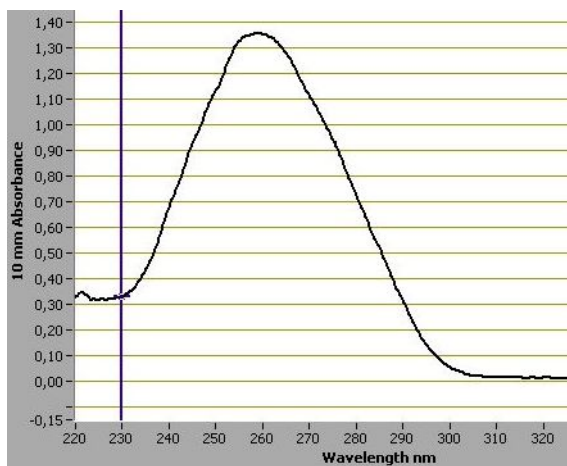

**Figure 2** Typical spectrum of pure DNA

### Agarose Gel Electrophoresis

- 1 Load 20 ng of gDNA for each sample in 10  $\mu$ L of DNase/RNase-free distilled water in the well of a single-comb Clear E-Gel (1.2% agarose, no stain). (You do not need to add loading buffer in this system).
- 2 As a control, load 20 ng of Human Reference DNA (Male and Female) or commercial Human Genomic DNA in 10  $\mu$ L of DNase/RNase-free distilled water in one of the wells of the E-Gel.
- 3 Mix 5  $\mu$ L of TrackIt 1 Kb DNA Ladder with 95  $\mu$ L of deionized water and load 10  $\mu$ L of the diluted ladder in one of the wells of the E-Gel.
- 4 Run the gel for 30 minutes as described in Invitrogen's instructions.
- 5 Open the gel cassette with E-Gel Opener as described in Invitrogen's instructions.
- 6 Stain the gel with SYBR Gold Nucleic Acid Gel Stain (diluted 1:10,000 by adding 10  $\mu$ L of SYBR Gold Nucleic Acid Gel Stain to 100 mL of DNase/RNase-free distilled water) in a plastic tray for 15 minutes.
- 7 Visualize the gel on the UV-transilluminator using a SYBR photographic filter.

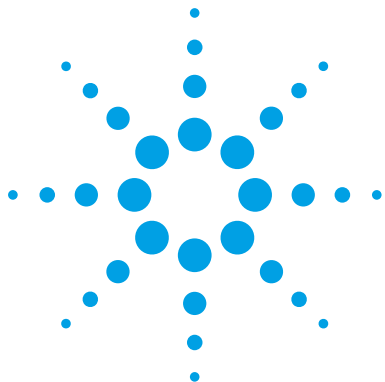

## 3 Sample Preparation

### Direct Method 38

Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit 40

### Amplification Method 43

Step 1. Fragmentation 45

Step 2. Library Preparation 46

Step 3. Amplification 47

Step 4. Purification of PCR products 48

Step 5. Quantitation of Amplified-Purified DNA 49

Step 6. Preparation of Amplified-Purified DNA before Labeling 49

This chapter describes the two Agilent recommended options to process gDNA prior to labeling.

You can choose between two methods for sample preparation prior to labeling: “Direct Method” on page 38 and “Amplification Method” on page 43. [Figure 1](#) on page 29 and [Figure 3](#) on page 44 show the respective workflows.

### CAUTION

The amplification method is not an option when you process SurePrint G3 CGH+SNP microarrays.



## Direct Method

### CAUTION

*For optimal performance, use high quality, intact template gDNA.* If the DNA isolation procedure described in this protocol cannot be followed, make sure that the DNA is free of RNA and protein contamination. If needed, repurify already isolated DNA and start from [step 6 on page 31](#) in the previous chapter.

Make sure that the gDNA is completely in solution by pipetting up and down. If needed, incubate at 37°C for 30 minutes. If the gDNA concentration > 350 ng/μL, dilute 1:2 in [Buffer AE](#) or [1×TE \(pH 8.0\)](#) and requantitate to make sure quantitation is accurate.

---

Use the Direct Method if you have at least 0.5 μg (for 1-, 2-, or 4-pack microarrays) or 0.2 μg (for 8-pack microarrays) of starting gDNA. You must use equal amounts of gDNA for both the experimental and reference channels. The required gDNA input amount and volume depends on the microarray format used and whether a restriction digestion is done before the labeling reaction (see [Table 20](#)).

### NOTE

For a wide variety of samples, high quality CGH microarray data is achieved when a restriction digestion step is used before the labeling step. But you can also achieve high quality data if you replace the restriction digestion step by a longer incubation at 98°C after you add the random primers in the labeling reaction step. See [“Step 1. Fluorescent Labeling of gDNA”](#) on page 52.

You cannot skip the restriction digestion step when you process SurePrint G3 CGH+SNP microarrays.

---

If you have 50 ng to <0.5 μg (for 1-, 2- or 4-pack microarrays) or <0.2 μg (for 8-pack microarrays) gDNA, see [“Amplification Method”](#) on page 43.

**Table 20** Requirement of gDNA Input Amount and Volume per Microarray<sup>\*</sup>

Microarray format	gDNA input amount requirement (µg)	Volume of gDNA with restriction digestion (µL)	Volume of gDNA without restriction digestion (µL)
1-pack	0.5 to 1.0	20.2	26
2-pack or 4-pack	0.5 to 1.0	20.2	26
8-pack	0.2 to 0.5	10.1	13

\* The gDNA requirement is the same for HD and G3 microarrays (e.g. 0.5 to 1.5 µg for both 4×44K and 4×180K microarrays).

### 3 Sample Preparation

#### Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit

## Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit

Both the SureTag Complete DNA Labeling Kit and the SureTag DNA Labeling Kit contain 10× Restriction Enzyme Buffer, BSA, Alu I and Rsa I.

### CAUTION

If a DNA concentration step is required before the restriction digestion, you must avoid carrying over high amounts of salt, EDTA, and contaminants to the restriction digestion reaction.

- 1 Equilibrate heat blocks or water baths to 37°C and 65°C or use a thermal cycler.
- 2 Thaw 10× Restriction Enzyme Buffer and BSA (included in the SureTag Complete DNA Labeling Kit and the SureTag DNA Labeling Kit). Flick the tube to briefly mix, and spin in a microcentrifuge.  
Store all reagents on ice while in use and return promptly to -20°C.
- 3 For each reaction, add the amount of gDNA to the appropriate nuclease-free tube or well in the PCR plate and add enough DNase/RNase-free distilled water to bring to the final volume listed in Table 20 on page 39.
- 4 Prepare the Digestion Master Mix by mixing the components in Table 21 or Table 22, based on the microarray format used, on ice in the order indicated. Mix well by pipetting up and down.



## Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit

**Table 21** Digestion Master Mix (for 1-pack, 2-pack and 4-pack microarrays)

Component	Per reaction (μL)	× 16 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)	× 96 rxns (μL) (including excess)
Nuclease-Free Water	2.0	34	100	200
10× Restriction Enzyme Buffer	2.6	44.2	130	260
BSA	0.2	3.4	10	20
Alu I	0.5	8.5	25	50
Rsa I	0.5	8.5	25	50
<b>Final volume of Digestion Master Mix</b>	<b>5.8</b>	<b>98.6</b>	<b>290</b>	<b>580</b>

**Table 22** Digestion Master Mix (for 8-pack microarrays)

Component	Per reaction (μL)	× 16 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)	× 96 rxns (μL) (including excess)
Nuclease-Free Water	1	17	50	100
10× Restriction Enzyme Buffer	1.3	22.1	65	130
BSA	0.1	1.7	5	10
Alu I	0.25	4.25	12.5	25
Rsa I	0.25	4.25	12.5	25
<b>Final volume of Digestion Master Mix</b>	<b>2.9</b>	<b>49.3</b>	<b>145</b>	<b>290</b>

- 5 Add 5.8 μL (for 1-, 2-, or 4-pack microarrays) or 2.9 μL (for 8-pack microarrays) of Digestion Master Mix to each reaction tube containing the gDNA to make a total volume of 26 μL (for 1-, 2-, or 4-pack microarrays) or 13 μL (for 8-pack microarrays). Mix well by pipetting up and down.

### 3 Sample Preparation

#### Restriction Digestion with the SureTag Complete DNA Labeling Kit or SureTag DNA Labeling Kit

- 6 Incubate the samples:
  - a Transfer sample tubes to a circulating water bath or heat block at 37°C. Incubate at 37°C for 2 hours.
  - b Transfer sample tubes to a circulating water bath or heat block at 65°C. Incubate at 65°C for 20 minutes to inactivate the enzymes.
  - c Move the sample tubes to ice.

*or*

Transfer sample tubes or plates to a thermal cycler. Program the thermal cycler according to [Table 23](#) and run the program:

**Table 23** Restriction digestion of the DNA using a thermal cycler

Step	Temperature	Time
Step 1	37°C	2 hours
Step 2	65°C	20 minutes
Step 3	4°C	hold

- 7 *Optional.* Take 2 µL of the digested gDNA and run on a 0.8% agarose gel stained with SYBR Gold to assess the completeness of the digestion. The majority of the digested products should be between 200 bp and 500 bp in length.
- 8 Proceed directly to “[Sample Labeling](#)” on page 51, or store digested gDNA for up to a month at -20°C.

*Do not do the restriction digestion steps in the next section, “[Amplification Method](#)”.*

## Amplification Method

### CAUTION

For optimal performance, use high quality, intact template gDNA. If the DNA isolation procedure described in this protocol cannot be followed, make sure that the DNA is free of RNA and protein contamination. If needed, repurify already isolated DNA and start from [step 6](#) on [page 31](#) in the previous chapter.

If you choose the amplification method, also amplify the reference DNA and make sure it is at a similar degree of intactness.

Make sure that the gDNA is completely in solution by pipetting up and down. If needed, incubate at 37°C for 30 minutes.

GenomePlex can be used on degraded samples if the extracted DNA is 500 bp or greater in size. However, greater quantities (up to 100 ng) of damaged DNA are required to get acceptable yield of final product. DNA isolated from FFPE samples is often severely degraded and damaged and is not always suitable for GenomePlex amplification.

*Do not use the amplification method to process SurePrint G3 CGH+SNP microarrays.*

---

Use the Amplification Method if you have limited amounts of gDNA. If you have 0.5 µg (for 1-, 2-, or 4-pack microarrays) or 0.2 µg (for 8-pack microarrays) or more gDNA, see “[Direct Method](#)” on [page 38](#).


### Reference

GenomePlex Whole Genome Amplification (WGA) Kit. Technical Bulletin. Sigma-Aldrich. 2006. TR/PHC 06/05-1

### Genomic Amplification

The Sigma GenomePlex Whole Genome Amplification (WGA) kit allows you to generate a representative amplification of gDNA. The kit uses a linker mediated primer PCR amplification technology based upon random fragmentation of gDNA and conversion of the resulting small fragments to PCR-amplifiable OmniPlex Library molecules flanked by universal priming sites. The OmniPlex library is then PCR amplified using universal oligonucleotide primers and a limited number of cycles. It is suitable to use with purified gDNA from a variety of sources including fresh frozen tissues and cultured cell lines.

### 3 Sample Preparation Amplification Method

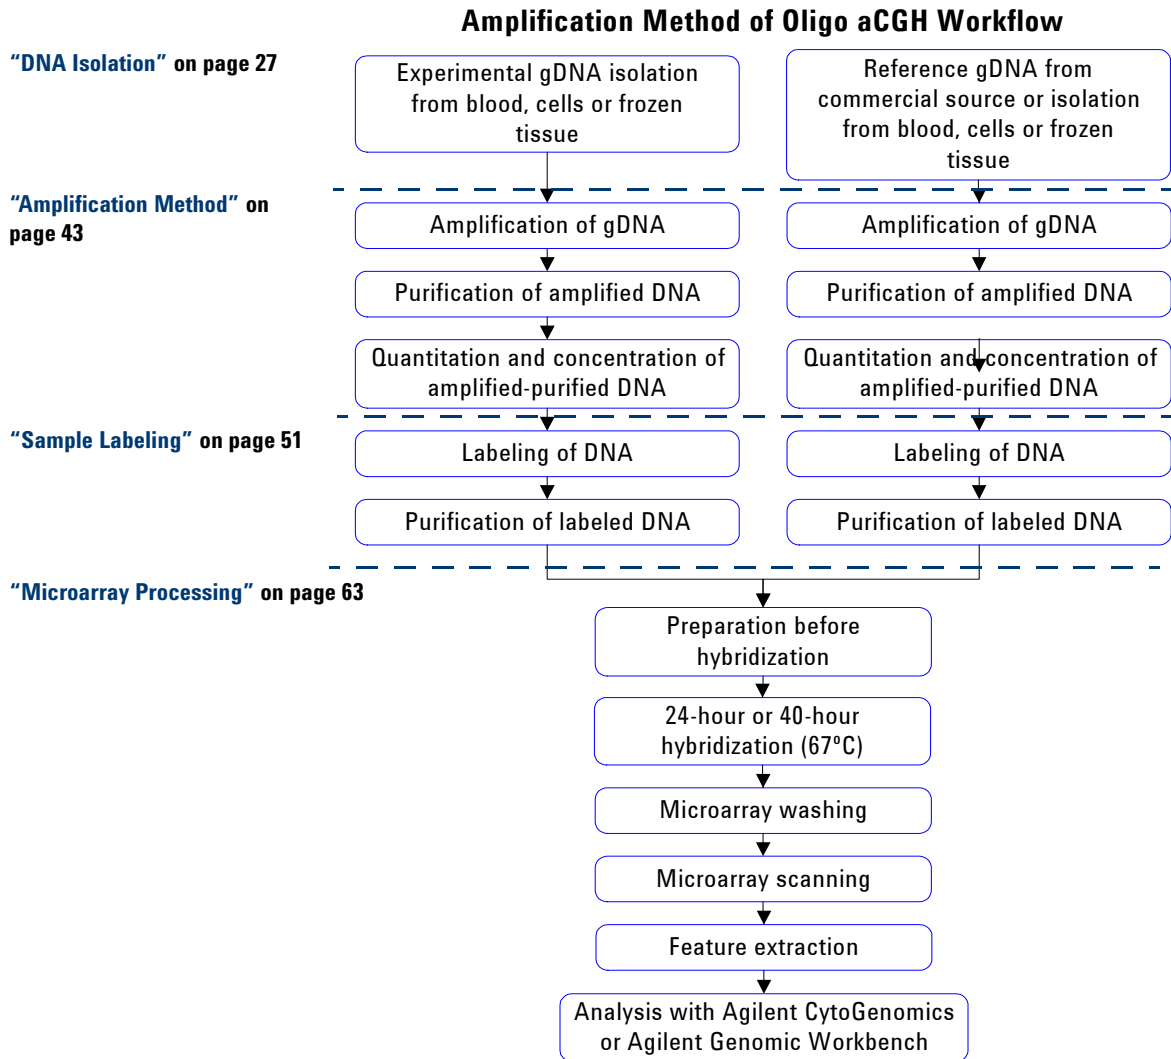

**Figure 3** Amplification workflow for sample preparation and microarray processing. Minimum of 50 ng of starting gDNA per sample is required.

This section describes Agilent recommended procedure to amplify gDNA using the Sigma GenomePlex Whole Genome Amplification (WGA) Kit (p/n WGA2).

## Step 1. Fragmentation

- 1 Add 50 ng of gDNA to a 200  $\mu$ L Thin-Wall Tube or plate. Add DNase/RNase-free distilled water to bring to a final volume of 10  $\mu$ L.
- 2 Add 1  $\mu$ L of 10 $\times$  Fragmentation Buffer to each reaction tube containing the gDNA to make a total volume of 11  $\mu$ L and mix well by pipetting up and down.
- 3 Place the tube or plate in a thermal cycler with heated lid at 95°C for *exactly* 4 minutes.

### CAUTION

The incubation is very time sensitive. Any deviation may alter results.

---

- 4 Immediately cool the sample on ice, then spin briefly in a centrifuge to drive the contents off the walls and lid.

### CAUTION

You must continue to “Step 2. Library Preparation” without interruption. The ends of the library DNA can degrade.

---

## Step 2. Library Preparation

- 1 Add 2  $\mu\text{L}$  of 1 $\times$  Library Preparation Buffer to each reaction tube.
- 2 Add 1  $\mu\text{L}$  of Library Stabilization Solution to each reaction tube.
- 3 Mix thoroughly, spin briefly in a centrifuge to drive the contents off the walls and lid and place in a thermal cycler with heated lid at 95°C for 2 minutes.
- 4 Cool the sample on ice, spin briefly in a centrifuge to drive the contents off the walls and lid, and return to ice.
- 5 Add 1  $\mu\text{L}$  Library Preparation Enzyme to make a total volume of 15  $\mu\text{L}$ . Mix thoroughly, and spin briefly in a centrifuge to drive the contents off the walls and lid.
- 6 Place sample in a thermal cycler and incubate as shown in Table 24.

**Table 24** Library Preparation Isothermal Reaction using thermal cycler (total time approximately 1 hour)

Temperature	Time (minutes)
16°C	20
24°C	20
37°C	20
75°C	5
4°C	Hold

- 7 Remove samples from the thermal cycler and spin briefly in a centrifuge to drive the contents off the walls and lid. Samples may be amplified immediately or stored at -20°C for up to three days.

## Step 3. Amplification

- 1 Prepare the **Amplification Master Mix** by mixing the components in **Table 25** on ice.

**Table 25** Amplification Master Mix

	Volume (μL)	x16 rxns (μL) including excess	x48 rxns (μL) including excess	x96 rxns (μL) including excess
10× Amplification Master Mix	7.5	127.5	375	750
Nuclease-Free Water	47.5	807.5	2,375	4,750
WGA DNA Polymerase	5	85	250	500
<b>Final volume of Amplification Master Mix</b>	<b>60</b>	<b>1,020</b>	<b>3,000</b>	<b>6,000</b>

- 2 Add 60 μL of **Amplification Master Mix** to each 15 μL reaction from the previous step to make a total volume of 75 μL.
- 3 Mix thoroughly, spin briefly in a centrifuge to drive the contents off the walls and lid, and place the samples in a thermal cycler with heated lid. Run the program below:

**Table 26** PCR Amplification (total time approximately 2 hours)

Step	Temperature	Time
Initial Denaturation	95°C	3 minutes
<b>Do 14 cycles as follows:</b>		
Denature	94°C	15 seconds
Anneal/Extend	65°C	5 minutes
After cycling	4°C	hold

- 4 Maintain the reactions at 4°C or store at -20°C for up to three days until ready for purification.

## Step 4. Purification of PCR products

Use **GenElute PCR Clean-Up Kit** for the purification of amplified DNA.

- 1** Before using for the first time, dilute the **Wash Solution Concentrate** with 48 ml of 100% **Ethanol**.
- 2** Insert a **GenElute plasmid mini spin column** (with a blue O-ring) into a **2 mL Collection Tube**, if not already assembled. Add 0.5 mL of the **Column Preparation Solution** to each **GenElute plasmid mini spin column** and spin in a centrifuge at  $12,000 \times g$  for 30 seconds to 1 minute. Discard the eluate, but keep the **2 mL Collection Tube**.

The **Column Preparation Solution** maximizes binding of the DNA to the membrane resulting in more consistent yields.

- 3** Add 375  $\mu\text{L}$  of **Binding Solution** to each 75  $\mu\text{L}$  sample. Transfer the solution into the **GenElute plasmid mini spin column**. Spin the column in a centrifuge at maximum speed ( $12,000$  to  $16,000 \times g$ ) for 1 minute. Discard the eluate, but keep the **2 mL Collection Tube**.
- 4** Place the binding column into the same collection tube. Apply 0.5 mL of diluted **Wash Solution Concentrate** to the column and spin in a centrifuge at maximum speed for 1 minute. Discard the eluate, but keep the **2 mL Collection Tube**.
- 5** Place the column into the same collection tube. Spin the column in a centrifuge at maximum speed for 2 minutes, without any additional wash solution, to remove excess ethanol. Discard any residual eluate as well as the **2 mL Collection Tube**.
- 6** Transfer the column to a fresh **2 mL Collection Tube**. Apply 50  $\mu\text{L}$  of **Elution Solution** to the center of each **GenElute plasmid mini spin column**. Incubate at room temperature for 1 minute.
- 7** To elute the DNA, spin the **GenElute plasmid mini spin column** in a centrifuge at maximum speed for 1 minute.

The PCR amplification product is now present in the eluate and is ready for quantitation and labeling without restriction enzyme digestion. The final amplified DNA can be stored at  $-20^{\circ}\text{C}$ .



## Step 5. Quantitation of Amplified-Purified DNA

Quantitate amplified-purified DNA using the NanoDrop ND-1000 UV-VIS Spectrophotometer or equivalent.

- 1 Select **Nucleic Acid Measurement**, then select **Sample Type** to be **DNA-50**.
- 2 Use 1.5  $\mu\text{L}$  of **Elution Solution** to blank the instrument.
- 3 Use 1.5  $\mu\text{L}$  of each purified DNA to measure DNA concentration. Record the DNA concentration ( $\text{ng}/\mu\text{L}$ ) for each sample.
- 4 Calculate the amplification yield ( $\mu\text{g}$ ) as

$$\text{Yield } (\mu\text{g}) = \frac{\text{DNA Concentration } (\text{ng}/\mu\text{L}) \times \text{Sample Volume } (\mu\text{L})}{1000 \text{ ng}/\mu\text{g}}$$

## Step 6. Preparation of Amplified-Purified DNA before Labeling

- 1 Add 2  $\mu\text{g}$  of amplified-purified DNA to a 1.5 mL RNase-free Microfuge Tube or well in the PCR plate and bring to a final volume of 26  $\mu\text{L}$  (1-, 2-, or 4-pack microarrays) or 13  $\mu\text{L}$  (8-pack microarrays) with DNase/RNase-free distilled water.


Both the experimental and reference channels require equal amounts of amplified-purified DNA for the subsequent labeling reaction.

- 2 If the DNA sample volume exceeds 26  $\mu\text{L}$  (for 1-pack, 2-pack, or 4-pack microarrays) or 13  $\mu\text{L}$  (for 8-pack microarrays), concentrate the amplified-purified DNA using a vacuum concentrator (such as a Speed Vac).

You can concentrate the DNA to dryness and resuspend in DNase/RNase-free distilled water. Do not excessively dry the DNA because the pellets will become difficult to resuspend.

Proceed directly to “Sample Labeling” on page 51 or store amplified-purified DNA at  $-20^{\circ}\text{C}$ . No restriction digestion step is needed.

**This page intentionally left blank.**

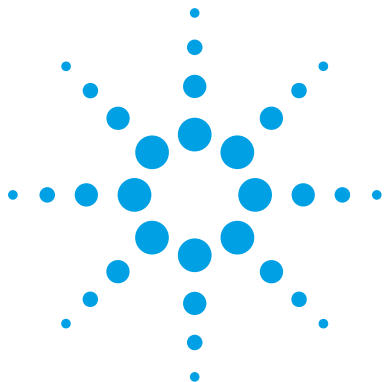

## 4 Sample Labeling

- Step 1. Fluorescent Labeling of gDNA 52
- Step 2. Purification of Labeled gDNA 56
- To determine yield, and degree of labeling or specific activity 61

The [SureTag Complete DNA Labeling Kit](#) and [SureTag DNA Labeling Kit](#) contain sufficient two-color labeling reaction reagents for:

- 25 1-pack, 2-pack, or 4-pack microarrays *or*
- 50 8-pack microarrays

Both the [SureTag Complete DNA Labeling Kit](#) and the [SureTag DNA Labeling Kit](#) contain clean-up columns for 25 reactions of each color. Order additional columns when processing more than 25 8-pack microarrays.

The kit uses random primers and the exo-Klenow fragment to differentially label gDNA samples with fluorescent-labeled nucleotides. For the Agilent Oligo aCGH application, the experimental sample is labeled with one dye while the reference sample is labeled with the other dye. The “polarity” of the sample labeling is a matter of experimental choice. Typically, the test sample is labeled with cyanine 5 and the reference with cyanine 3.



## Step 1. Fluorescent Labeling of gDNA

### NOTE

Cyanine 3-dUTP and cyanine 5-dUTP are light sensitive and are subject to degradation by multiple freeze thaw cycles. Minimize light exposure throughout the labeling procedure.

### CAUTION

The test/reference sample pairs must be treated identically when they are processed, or else the quality of your data can be adversely affected. The best way to ensure that the sample pairs are exposed to the same temperature during the denaturation step is to use a water bath.

- 1 Equilibrate heat blocks or water baths to 98°C, 37°C and 65°C, or use a thermal cycler.
- 2 Spin the samples in a centrifuge for 1 minute at 6,000 × g to drive the contents off the walls and lid.
- 3 Add **Random Primer**:
  - For 1-pack, 2-pack, and 4-pack microarrays, add 5 µL of **Random Primer** to each reaction tube containing 26 µL of gDNA to make a total volume of 31 µL (or 24 µL of gDNA to make a total volume of 29 µL if the optional agarose gel step on [page 42](#) was done). Mix well by pipetting up and down gently.
  - For 8-pack microarrays, add 2.5 µL of **Random Primer** to each reaction tube that contains 13 µL of gDNA to make a total volume of 15.5 µL (or 11 µL of gDNA to make a total volume of 13.5 µL if the optional agarose gel step on [page 42](#) was done). Mix well by pipetting up and down gently.
- 4 Transfer sample tubes to a circulating water bath or heat block at 98°C. Incubate at 98°C for 3 minutes (with restriction digestion) or 10 minutes (without restriction digestion), then move to ice and incubate on ice for 5 minutes.

*or*

Transfer sample tubes to a thermal cycler. Program the thermal cycler according to [Table 27](#) and run the program.

**Table 27** DNA denaturation and fragmentation using a thermal cycler

Step	Temperature	Time (with restriction digestion)	Time (without restriction digestion)
Step 1	98°C	3 minutes	10 minutes
Step 2	4°C	hold	hold

5 Spin the samples in a centrifuge for 1 minute at 6,000 × g to drive the contents off the walls and lid.

6 For 1-pack, 2-pack and 4-pack microarrays:

- a Mix the components in [Table 28](#) on ice in the order indicated to prepare one cyanine-3 and one cyanine-5 [Labeling Master Mix](#).

**Table 28** Labeling Master Mix (for 1-pack, 2-pack and 4-pack microarrays)

Component	Per reaction (μL)	× 8 rxns (μL) (including excess)	× 24 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)
Nuclease-Free Water	2.0*	17*	50*	100*
5× Reaction Buffer	10.0	85	250	500
10× dNTPs	5.0	42.5	125	250
Cyanine 3-dUTP <i>or</i> Cyanine 5-dUTP	3.0	25.5	75	150
Exo (-) Klenow	1.0	8.5	25	50
<b>Final volume of Labeling Master Mix</b>	<b>19.0 or 21.0*</b>	<b>161.5 or 178.5*</b>	<b>475 or 525*</b>	<b>950 or 1050*</b>

\* Do *not* add [Nuclease-Free Water](#) if you skipped the optional agarose gel step ([step 7](#) on [page 42](#)).

- b Add 19 μL (or 21 μL) of [Labeling Master Mix](#) to each reaction tube containing the gDNA to make a total volume of 50 μL. Mix well by gently pipetting up and down.

## 4 Sample Labeling

### Step 1. Fluorescent Labeling of gDNA

7 For 8-pack microarrays:

- a Mix the components in [Table 29](#) on ice in the order indicated to prepare one cyanine-3 and one cyanine-5 [Labeling Master Mix](#).

**Table 29** Labeling Master Mix (for 8-pack microarrays)

Component	Per reaction (μL)	× 8 rxns (μL) (including excess)	× 24 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)
Nuclease-Free Water*	2.0*	17*	50*	100*
5× Reaction Buffer	5.0	42.5	125	250
10× dNTPs	2.5	21.25	62.5	125
Cyanine 3-dUTP <i>or</i> Cyanine 5-dUTP	1.5	12.75	37.5	75
Exo (-) Klenow	0.5	4.25	12.5	25
<b>Final volume of Labeling Master Mix</b>	<b>9.5 or 11.5*</b>	<b>80.75 or 97.75*</b>	<b>237.5 or 287.5*</b>	<b>475 or 575*</b>

\* Do *not* add [Nuclease-Free Water](#) if you skipped the optional agarose gel step ([step 7](#) on [page 42](#)).

- b Add 9.5 μL (or 11.5 μL) of [Labeling Master Mix](#) to each reaction tube that contains the gDNA to make a total volume of 25 μL. Mix well by gently pipetting up and down.

8 Incubate the samples:

- a Transfer sample tubes to a circulating water bath or heat block at 37°C. Incubate at 37°C for 2 hours.
- b Transfer sample tubes to a circulating water bath or heat block at 65°C. Incubate at 65°C for 10 minutes to inactivate the enzyme.
- c Move the sample tubes to ice.

*or*

Transfer sample tubes to a thermal cycler. Program the thermal cycler according to [Table 30](#) and run the program.

**Table 30** DNA labeling using a thermal cycler

Step	Temperature	Time
Step 1	37°C	2 hours
Step 2	65°C	10 minutes
Step 3	4°C	hold

Reactions can be stored up to a month at -20°C in the dark.

## Step 2. Purification of Labeled gDNA

Labeled gDNA is purified using the reaction [Purification Column](#) provided with the [SureTag Complete DNA Labeling Kit](#) and [SureTag DNA Labeling Kit](#). The [Purification Column](#) includes:

- column
- 2-mL collection tube

For high-throughput, labeled gDNA can be purified using individual [AutoScreen A, 96-well plate](#) from GE Healthcare. See “[GE Healthcare 96-Well Plates High-Throughput Option](#)” on page 58.

### NOTE

Keep cyanine-3 and cyanine-5 labeled gDNA samples separated throughout this clean-up step.

### Agilent Purification Columns

- 1 Spin the labeled gDNA samples in a centrifuge for 1 minute at  $6,000 \times g$  to drive the contents off the walls and lid.
- 2 Add 430  $\mu\text{L}$  of [1 \$\times\$ TE \(pH 8.0\)](#) to each reaction tube.
- 3 For each gDNA sample to be purified, place a [column](#) into a [2-mL collection tube](#) and label the [column](#) appropriately. Load each labeled gDNA onto a [column](#).
- 4 Cover the [column](#) with a cap and spin for 10 minutes at  $14,000 \times g$  in a microcentrifuge at room temperature. Discard the flow-through and place the [column](#) back in the [2-mL collection tube](#).
- 5 Add 480  $\mu\text{L}$  of [1 \$\times\$ TE \(pH 8.0\)](#) to each [column](#). Spin for 10 minutes at  $14,000 \times g$  in a microcentrifuge at room temperature. Discard the flow-through.
- 6 Invert the [column](#) into a fresh [2-mL collection tube](#) that has been appropriately labeled. Spin for 1 minute at  $1,000 \times g$  in a microcentrifuge at room temperature to collect purified sample.  
The volume per sample will be approximately 20 to 32  $\mu\text{L}$ .
- 7 Add [1 \$\times\$ TE \(pH 8.0\)](#), or use a concentrator to bring the sample volume to that listed in [Table 31](#). Do not excessively dry the gDNA because the pellets will become difficult to resuspend.



- 8 Mix thoroughly. If the sample has dried or precipitated after concentration, incubate the tube that contains gDNA sample on ice for 5 minutes, and then pipette the solution up and down 10 times.
- 9 Take 1.5  $\mu\text{L}$  of each sample to determine yield and specific activity. See “To determine yield, and degree of labeling or specific activity” on page 61. Refer to Table 33 on page 62 for expected yield of labeled gDNA and specific activity after labeling and clean-up, when starting with high quality gDNA.
- 10 In a fresh 1.5 mL RNase-free Microfuge Tube or 200  $\mu\text{L}$  Thin-Wall Tube, combine test and reference sample using the appropriate cyanine-5-labeled sample and cyanine-3-labeled sample for a total mixture volume listed in Table 31. Use the appropriate container listed in Table 31.  
Labeled DNA can be stored up to one month at  $-20^{\circ}\text{C}$  in the dark.

**Table 31** Sample volume and total mixture volumes

Microarray	Cyanine 3 or Cyanine 5 sample volume after purification	Total mixture volume after Nanodrop and combining	Container
1-pack	80.5 $\mu\text{L}$	158 $\mu\text{L}$	1.5 mL RNase-free Microfuge Tube
2-pack	41 $\mu\text{L}$	79 $\mu\text{L}$	1.5 mL RNase-free Microfuge Tube or Tall Chimney PCR plate
4-pack	21 $\mu\text{L}$	39 $\mu\text{L}$	1.5 mL RNase-free Microfuge Tube, Tall Chimney PCR plate, or 96-well PCR plate
8-pack	9.5 $\mu\text{L}$	16 $\mu\text{L}$	1.5 mL RNase-free Microfuge Tube or Tall Chimney PCR plate, or 96-well PCR plate

## GE Healthcare 96-Well Plates High-Throughput Option

### NOTE

Use the same centrifuge speed and length for all three spinning steps (step 4, step 7 and step 11). If you spin only one plate, make sure that you counterbalance.

For 1-pack, 2-pack, 4-pack, you can use two wells of the [AutoScreen A, 96-well plate](#) per sample, or concentrate the samples down to 25  $\mu\text{L}$  with a vacuum concentrator (such as a Speed Vac).

**1** Get two [96-well PCR plates](#). Label one each as:

- wash plate
- collection plate

The [wash plate](#) can be reused in next experiments.

**1** Remove the [AutoScreen A, 96-well plate](#) from the foil storage pouch.

If the [AutoScreen A, 96-well plate](#) were stored at 4°C, allow them to equilibrate to ambient temperature before use (approximately two hours).

**2** Carefully remove the top and bottom seal of the [AutoScreen A, 96-well plate](#).

Once the bottom seal is removed, keep the [AutoScreen A, 96-well plate](#) on top of a [wash plate](#). Do not allow the bottom surface to come in contact with laboratory bench top liners, wipes, or other materials.

**3** Place the purification plates in reusable [wash plates](#).

**4** Spin the purification plates in a centrifuge for 5 minutes at  $910 \times g$ .

**5** Discard the flow-through from the [wash plates](#), and place the [AutoScreen A, 96-well plate](#) back to the same [wash plates](#).

**6** Add 150  $\mu\text{L}$  of DNase/RNase-free distilled water to the [AutoScreen A, 96-well plate](#).

**7** Spin again in a centrifuge for 5 minutes at  $910 \times g$ .

**8** Discard the flow-through.

**9** Transfer the [AutoScreen A, 96-well plate](#) to the sample collection plate.

**10** Add labeled gDNA to the [AutoScreen A, 96-well plate](#):

- For 1-pack, 2-pack, 4-pack microarray samples that were not concentrated to 25  $\mu\text{L}$ , add  $2 \times 25 \mu\text{L}$  labeled gDNA to two separate wells.

- For 1-pack, 2-pack, 4-pack microarray samples that were concentrated to 25  $\mu\text{L}$  with concentrator and for 8-pack microarray samples, add 1 $\times$ 25  $\mu\text{L}$  labeled gDNA to one well.
- 11** Spin in a centrifuge for 5 minutes at  $910 \times g$  to collect the purified labeled gDNA in the sample collection plate. The volume per sample will be approximately 20  $\mu\text{L}$ .
  - 12** For 1-pack, 2-pack and 4-pack microarray samples that were not concentrated prior to purification, combine the duplicate samples for a total volume of approximately 40  $\mu\text{L}$ .
  - 13** Take 1.5  $\mu\text{L}$  of each sample to determine the yield and specific activity. See “To determine yield, and degree of labeling or specific activity” on page 61. Refer to Table 33 on page 62 for expected yield of labeled gDNA and specific activity after labeling and clean-up, when starting with high quality gDNA.
  - 14** Combine the test and reference sample using the appropriate cyanine 5-labeled sample and cyanine-3-labeled sample. Use the appropriate container listed in Table 32. Add 1 $\times$ TE (pH 8.0) or use a concentrator to bring to the Total Mixture Volume in Table 32.

If needed, you can concentrate the combined cyanine 5- and cyanine 3-labeled gDNA mixture to dryness and resuspend in 1 $\times$ TE (pH 8.0) to the final volume listed in Table 32. Do not excessively dry the samples because the pellets will become difficult to resuspend.

## 4 Sample Labeling

### Step 2. Purification of Labeled gDNA

**Table 32** Total mixture volumes

Micro array	Treatment prior to purification	Cy3 or Cy5 sample volume after purification	Volume after Nanodrop and combining	1× TE volume	Total mixture volume	Container
1-pack	without vacuum concentration*	40 µL	77 µL	81 µL	158 µL	1.5 mL RNase-free Microfuge Tube
	with vacuum concentration	20 µL	37 µL	121 µL	158 µL	1.5 mL RNase-free Microfuge Tube
2-pack	without vacuum concentration*	40 µL	77 µL	2 µL	79 µL	1.5 mL RNase-free Microfuge Tube or Tall Chimney PCR plate
	with vacuum concentration	20 µL	37 µL	42 µL	79 µL	1.5 mL RNase-free Microfuge Tube or Tall Chimney PCR plate
4-pack	without vacuum concentration*	40 µL	77 µL	0 µL <sup>†</sup>	39 µL	1.5 mL RNase-free Microfuge Tube, Tall Chimney PCR plate, or 96-well PCR plate
	with vacuum concentration	20 µL	37 µL	2 µL	39 µL	1.5 mL RNase-free Microfuge Tube, Tall Chimney PCR plate, or 96-well PCR plate
8-pack	without vacuum concentration	20 µL	37 µL	0 µL <sup>†</sup>	16 µL	1.5 mL RNase-free Microfuge Tube, Tall Chimney PCR plate, or 96-well PCR plate

\* You will use 2 wells of the purification plate per sample.

† Concentrate the sample to the volume indicated in the Total Mixture Volume column.

## To determine yield, and degree of labeling or specific activity

Use the NanoDrop 8000 or 2000 UV-VIS Spectrophotometer to measure yield, and degree of labeling or specific activity.

- 1 From the main menu, select **MicroArray Measurement**, then from the **Sample Type** menu, select **DNA-50**.
- 2 Use 1.5  $\mu\text{L}$  of **1 $\times$ TE (pH 8.0)** to blank the instrument.
- 3 Use 1.5  $\mu\text{L}$  of purified labeled gDNA for quantitation. Measure the absorbance at  $A_{260\text{nm}}$  (DNA),  $A_{550\text{nm}}$  (cyanine 3), and  $A_{650\text{nm}}$  (cyanine 5).
- 4 Calculate the Degree of Labeling or Specific Activity of the labeled gDNA:

$$\text{Degree of Labeling} = \frac{340 \times \text{pmol per } \mu\text{L dye}}{\text{ng per } \mu\text{L gDNA} \times 1000} \times 100\%$$

$$\text{Specific Activity}^* = \frac{\text{pmol per } \mu\text{L of dye}}{\mu\text{g per } \mu\text{L gDNA}}$$

\*pmol dyes per  $\mu\text{g}$  gDNA

The Specific Activity is Degree of Labeling divided by 0.034.

- 5 Record the gDNA concentration ( $\text{ng}/\mu\text{L}$ ) for each sample. Calculate the yield as

$$\text{Yield } (\mu\text{g}) = \frac{\text{DNA Concentration } (\text{ng}/\mu\text{L}) \times \text{Sample Volume } (\mu\text{L})}{1000 \text{ ng}/\mu\text{g}}$$

Refer to [Table 33](#) and for expected yield of labeled gDNA and specific activity after labeling and purification, when starting with high quality gDNA.

## 4 Sample Labeling

To determine yield, and degree of labeling or specific activity


**Table 33** Expected Yield and Specific Activity after Labeling and Clean-up

Input gDNA ( $\mu\text{g}$ )	Yield ( $\mu\text{g}$ )	Specific Activity of Cyanine 3 Labeled Sample ( $\text{pmol}/\mu\text{g}$ )	Specific Activity of Cyanine 5 Labeled Sample ( $\text{pmol}/\mu\text{g}$ )
0.2 <sup>*</sup>	3 to 5	20 to 25	15 to 25
0.5	8 to 11	20 to 35	20 to 30
1	9 to 12	25 to 40	20 to 35

<sup>\*</sup> Half labeling reaction for 8-pack microarrays (half the amount of random primers, dye, enzyme, and dNTPs)

If you replaced the restriction digestion step by a longer incubation at 98°C, the specific activity of cyanine 3 and -5 labeled sample will be about 5 pmol/ $\mu\text{g}$  lower than the values indicated in [Table 33](#). The Yield after labeling and the signal to noise of the microarrays will be the same.

The cyanine-3 and cyanine-5 yield after labeling should be the same. If not, refer to “[Troubleshooting](#)” on page 89.

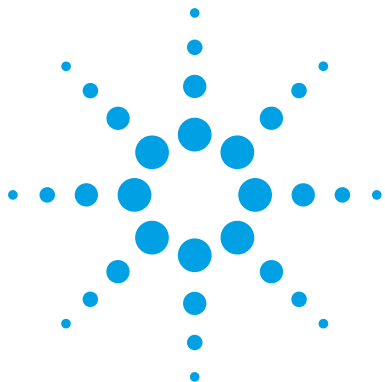

## 5 Microarray Processing

Hybridization	64
Microarray Wash	70
Microarray Scanning and Analysis	81

Microarray processing consists of hybridization, washing, and scanning.



## Hybridization

If you are new to microarray processing, refer to the “Running a microarray experiment” training presentation, which you can find when you go to <http://www.genomics.agilent.com> and search on the title of the presentation (“Running a microarray experiment”). This presentation shows you how to hybridize, wash and scan microarray slides.

To practice hybridization, prepare a 1:1 2× HI-RPM Hybridization Buffer and water mix and use a microscope slide or used microarray slide, and a gasket slide. You can use the same slide to practice wash and placement of slide in the slide holder.

Before you begin, make sure you read and understand “Microarray Handling Tips” on page 101.

### Step 1. Prepare the 10× Blocking Agent

- 1 Add 1,350 µL of DNase/RNase-free distilled water to the vial containing lyophilized 10× aCGH Blocking Agent (included in the Oligo aCGH/ChIP-on-chip Hybridization Kit).
- 2 Leave at room temperature for 60 minutes and mix on a vortex mixer to reconstitute sample before use or storage.

#### NOTE

The 10× Blocking Agent can be prepared in advance and stored at -20°C.



## Step 2. Prepare labeled gDNA for hybridization

- 1 Equilibrate water baths or heat blocks to 98°C and 37°C or use a thermal cycler.
- 2 Mix the components according to the microarray format to prepare the Hybridization Master Mix.

**Table 34** Hybridization Master Mix for **1-pack** microarray

Component	Volume (μL) per hybridization	× 8 rxns (μL) (including excess)	× 24 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)
Cot-1 DNA (1.0 mg/mL) <sup>*</sup>	50	425	1,250	2,500
10× aCGH Blocking Agent <sup>†</sup>	52	442	1,300	2,600
2× HI-RPM Hybridization Buffer <sup>†</sup>	260	2,210	6,500	13,000
Final Volume of Hybridization Master Mix	362	3,077	9,050	18,100

<sup>\*</sup> Use Cot-1 DNA (1.0 mg/mL) from the appropriate species.

<sup>†</sup> Included in the Oligo aCGH/ChIP-on-chip Hybridization Kit

**Table 35** Hybridization Master Mix for **2-pack** microarray

Component	Volume (μL) per hybridization	× 8 rxns (μL) (including excess)	× 24 rxns (μL) (including excess)	× 48 rxns (μL) (including excess)
Cot-1 DNA (1.0 mg/mL) <sup>*</sup>	25	212.5	625	1,250
10× aCGH Blocking Agent <sup>†</sup>	26	221	650	1,300
2× HI-RPM Hybridization Buffer <sup>†</sup>	130	1,105	3,250	6,500
Final Volume of Hybridization Master Mix	181	1,538.5	4,525	9,050

<sup>\*</sup> Use Cot-1 DNA (1.0 mg/mL) from the appropriate species.

<sup>†</sup> Included in the Oligo aCGH/ChIP-on-chip Hybridization Kit

## 5 Microarray Processing

### Step 2. Prepare labeled gDNA for hybridization

**Table 36** Hybridization Master Mix for **4-pack** microarray

Component	Volume (µL) per hybridization	× 8 rxns (µL) (including excess)	× 24 rxns (µL) (including excess)	× 48 rxns (µL) (including excess)
Cot-1 DNA (1.0 mg/mL) <sup>*</sup>	5	42.5	125	250
10× aCGH Blocking Agent <sup>†</sup>	11	93.5	275	550
2× HI-RPM Hybridization Buffer <sup>†</sup>	55	467.5	1,375	2,750
Final Volume of Hybridization Master Mix	71	603.5	1,775	3,550

<sup>\*</sup> Use Cot-1 DNA (1.0 mg/mL) from the appropriate species.

<sup>†</sup> Included in the Oligo aCGH/ChIP-on-chip Hybridization Kit

**Table 37** Hybridization Master Mix for **8-pack** microarray

Component	Volume (µL) per hybridization	× 8 rxns (µL) (including excess)	× 24 rxns (µL) (including excess)	× 48 rxns (µL) (including excess)
Cot-1 DNA (1.0 mg/mL) <sup>*</sup>	2	17	50	100
10× aCGH Blocking Agent <sup>†</sup>	4.5	38.25	112.5	225
2× HI-RPM Hybridization Buffer <sup>†</sup>	22.5	191.25	562.5	1,125
Final Volume of Hybridization Master Mix	29	246.5	725	1,450

<sup>\*</sup> Use Cot-1 DNA (1.0 mg/mL) from the appropriate species.

<sup>†</sup> Included in the Oligo aCGH/ChIP-on-chip Hybridization Kit

- 3 Add the appropriate volume of the Hybridization Master Mix to the 1.5 mL RNase-free Microfuge Tube, Tall Chimney PCR plate well or 96-well PCR plate well that contains the labeled gDNA to make the total volume listed in Table 38.

**Table 38** Volume of Hybridization Master Mix per hybridization

Microarray format	Volume of Hybridization Master Mix	Total volume
1-pack	362 $\mu$ L	520 $\mu$ L
2-pack	181 $\mu$ L	260 $\mu$ L
4-pack	71 $\mu$ L	110 $\mu$ L
8-pack	29 $\mu$ L	45 $\mu$ L

- 4 Mix the sample by pipetting up and down, then quickly spin in a centrifuge to drive contents to the bottom of the reaction tube.
- 5 Transfer sample tubes to a circulating water bath or heat block at 98°C. Incubate at 98°C for 3 minutes, then immediately transfer sample tubes to a circulating water bath or heat block at 37°C. Incubate at 37°C for 30 minutes.

*or*

Transfer sample tubes to a thermal cycler. Program the thermal cycler according to the following table and run the program:

**Table 39** Thermal cycler program

Step	Temperature	Time
Step 1	98°C	3 minutes exactly
Step 2	37°C	30 minutes

- 6 Remove sample tubes from the water bath, heat block, or thermal cycler. Spin 1 minute at 6000  $\times$  g in a centrifuge to collect the sample at the bottom of the tube.

The samples are ready to be hybridized.

### CAUTION

The samples must be hybridized immediately. If not, keep the temperature of hybridization sample mixtures as close to 37°C as possible on a heat block, thermal cycler or in an oven.

### Step 3. Prepare the hybridization assembly

Refer to the *Agilent Microarray Hybridization Chamber User Guide* (G2534-90001) for in-depth instructions on how to load samples, assemble and disassemble chambers, as well as other helpful tips. This user guide can be downloaded from the Agilent Web site at [www.agilent.com/chem/dnamanuals-protocols](http://www.agilent.com/chem/dnamanuals-protocols).

Before you begin, make sure you read and understand “[Microarray Handling Tips](#)” on page 101.

- 1 Load a clean gasket slide into the Agilent SureHyb chamber base with the gasket label facing up and aligned with the rectangular section of the chamber base. Ensure that the gasket slide is flush with the chamber base and is not ajar.
- 2 Slowly dispense hybridization sample mixture onto the gasket well in a “drag and dispense” manner:
  - 490  $\mu\text{L}$  (for 1-pack microarray)
  - 245  $\mu\text{L}$  (for 2-pack microarray)
  - 100  $\mu\text{L}$  (for 4-pack microarray)
  - 40  $\mu\text{L}$  (for 8-pack microarray)

For multi-pack microarray formats (2-pack, 4-pack or 8-pack microarray), load all gasket wells before you load the microarray slide. For multi-pack formats, refer to “[Agilent Microarray Layout and Orientation](#)” on page 102.

#### CAUTION

Keep the temperature of hybridization sample mixtures as close to 37°C as possible. To do this, process them in small batches and/or put them on a heat block, thermal cycler or in an oven.

- 3 Put a microarray slide “active side” down onto the gasket slide, so the numeric barcode side is facing up and the “Agilent”-labeled barcode is facing down. Assess that the sandwich-pair is properly aligned.
- 4 Put the SureHyb chamber cover onto the sandwiched slides and slide the clamp assembly onto both pieces.
- 5 Hand-tighten the clamp firmly onto the chamber.

- 6 Vertically rotate the assembled chamber to wet the slides and assess the mobility of the bubbles. Tap the assembly on a hard surface if necessary to move stationary bubbles.

## Step 4. Hybridize

- 1 Load each assembled chamber into the oven rotator rack. Start from the center of the rack (position 3 or 4 when counting from the left). Set your hybridization rotator to rotate at 20 rpm.
- 2 Hybridize at 67°C for:
  - 24 hours (4-pack and 8-pack microarrays)
  - 40 hours (1-pack and 2-pack microarrays)

### CAUTION

If you are not loading all the available positions on the hybridization rotator rack, be sure to *balance* the loaded hybridization chambers on the rack similar to a centrifuge to prevent unnecessary strain on the oven motor.

---

### CAUTION

You must calibrate the hybridization oven regularly for accuracy of the collected data. Refer to *Agilent G2545A Hybridization Calibration Procedure* (p/n G2545-90002) for more information.

---

For more information on the effects of hybridization temperature and time, as well as the rotation speed on the final microarray results, please refer to the application note titled “60-mer Oligo-Based Comparative Genomic Hybridization” (publication 5989-4848EN) from the Agilent Web site at [www.agilent.com/chem/dnaapplications](http://www.agilent.com/chem/dnaapplications).

### NOTE

The [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#) that is used in the microarray wash procedure needs to be warmed overnight. While you are waiting for the microarray slides to hybridize, do the steps in “[Step 1. Prewarm Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 \(overnight\)](#)” on page 71.

---

## Microarray Wash

### NOTE

The microarray wash procedure must be done in environments where ozone levels are 5 ppb or less. For Scanner C and Scanner B, if ozone levels are between 5 to 10 in your laboratory, use the Agilent Ozone Barrier Slide Cover. SureScan microarray scanner uses a slide holder with a built-in ozone barrier. If ozone levels exceed 10 ppb, use the [Stabilization and Drying Solution](#) together with the ozone barrier.

You can also use Carbon Loaded Non-woven Filters to remove ozone from the air. These filters can be installed in either your HVAC system, or as part of small Ozone Controlled Enclosures. These free-standing enclosures can be installed either on a lab bench or as a walk-in room within your lab. These products are available through filter suppliers listed in Agilent Technical Note 5989-0875EN.

Before you begin, determine which wash procedure to use:

**Table 40** Wash procedure to follow

Ozone level in your lab	Wash Procedure	Ozone-Barrier Slide Cover
< 5 ppb	"Wash Procedure A (without Stabilization and Drying Solution)" on page 74	No
> 5 ppb < 10 ppb	"Wash Procedure A (without Stabilization and Drying Solution)" on page 74	Yes
> 10 ppb	"Wash Procedure B (with Stabilization and Drying Solution)" on page 76	Yes

### CAUTION

Do not use detergent to wash the staining dishes as some detergents may leave fluorescent residue on the dishes. If you do, you must ensure that all traces are removed by thoroughly rinsing with [Milli-Q ultrapure water](#).

- Always use clean equipment when conducting the wash procedures.
- Use only dishes that are designated and dedicated for use in Agilent oligo aCGH experiments.

## Step 1. Prewarm Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 (overnight)

**Step 1. Prewarm Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 (overnight)**

The temperature of Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 must be at 37°C for optimal performance.

- 1 Add the volume of buffer required to a Sterile storage bottle and warm overnight in an incubator or circulating water bath set to 37°C.
- 2 Put a slide-staining dish with a lid, a 1.5 L glass dish, and one to two liters of Milli-Q ultrapure water in an incubator or water bath set at 37°C to warm overnight.

**Step 2. Wash with Milli-Q ultrapure water**

Rinse slide-staining dishes, slide racks and stir bars thoroughly with high-quality Milli-Q ultrapure water before use and in between washing groups.

- 1 Run copious amounts of Milli-Q ultrapure water through the slide-staining dishes, slide racks and stir bars.
- 2 Empty out the water collected in the dishes at least five times.
- 3 Repeat step 1 and step 2 until all traces of contaminating material are removed.

### Step 3. Clean with Acetonitrile (Wash Procedure B Only)

Acetonitrile wash removes any remaining residue of [Stabilization and Drying Solution](#) from slide-staining dishes, slide racks and stir bars that were used in previous experiments with “[Wash Procedure B \(with Stabilization and Drying Solution\)](#)” on page 76.

#### WARNING

Do **Acetonitrile** washes in a vented fume hood. **Acetonitrile** is highly flammable and toxic.

- 1 Add the slide rack and stir bar to the slide-staining dish, and transfer to a magnetic stir plate.
- 2 Fill the slide-staining dish with 100% [Acetonitrile](#).
- 3 Turn on the magnetic stir plate and adjust the speed to a setting of 4 (medium speed).
- 4 Wash for 5 minutes at room temperature.
- 5 Discard the [Acetonitrile](#) as is appropriate for your site.
- 6 Repeat [step 1](#) through [step 5](#).
- 7 Air dry everything in the vented fume hood.
- 8 Continue with the [Milli-Q ultrapure water](#) wash as previously instructed.

### Step 4. Prewarm Stabilization and Drying Solution (Wash Procedure B Only)

The [Stabilization and Drying Solution](#) contains an ozone scavenging compound dissolved in [Acetonitrile](#). The compound in solution is present in saturating amounts and may precipitate from the solution under normal storage conditions. If the solution shows visible precipitation, warming of the solution will be necessary to redissolve the compound. Washing slides using [Stabilization and Drying Solution](#) showing visible precipitation will have profound adverse effects on microarray performance.



## Step 4. Prewarm Stabilization and Drying Solution (Wash Procedure B Only)

**WARNING**

The **Stabilization and Drying Solution** is a flammable liquid. Warming the solution will increase the generation of ignitable vapors. Use gloves and eye/face protection in every step of the warming procedures.

---

**WARNING**

Do not use a hot plate, oven, an open flame or a microwave. Do not increase temperature rapidly. Warm and mix the material away from ignition sources.

---

**WARNING**

Failure to follow the outlined process will increase the potential for fire, explosion, and possible personal injury.

---

- 1 Put a clean magnetic stir bar into the **Stabilization and Drying Solution** bottle and recap.
- 2 Partially fill a plastic bucket with hot water at approximately 40°C to 45°C (for example from a hot water tap).
- 3 Put the **Stabilization and Drying Solution** bottle into the hot water in the plastic bucket.
- 4 Put the plastic bucket on a magnetic stirrer (*not a hot-plate*) and stir.
- 5 The hot water cools to room temperature. If the precipitate has not all dissolved replenish the cold water with hot water.
- 6 Repeat [step 5](#) until the solution is clear.
- 7 After the precipitate is completely dissolved, allow the solution to equilibrate to room temperature prior to use.

**CAUTION**

Do not filter the **Stabilization and Drying Solution**, or the concentration of the ozone scavenger may vary.

---

## Step 5. Wash microarrays

### Wash Procedure A (*without Stabilization and Drying Solution*)

Always use fresh Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 and Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 for each wash group (up to five slides).

Table 41 lists the wash conditions for the Wash Procedure A without Stabilization and Drying Solution.

**Table 41** Wash conditions

	Dish	Wash buffer	Temperature	Time
Disassembly	#1	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1	Room temperature	
1st wash	#2	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1	Room temperature	5 minutes
2nd wash	#3	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2	37°C	1 minute

- 1 Completely fill slide-staining dish #1 with Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 at room temperature.
- 2 Prepare dish #2:
  - a Put a slide rack into slide-staining dish #2.
  - b Add a magnetic stir bar. Fill slide-staining dish #2 with enough Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 at room temperature to cover the slide rack.
  - c Put this dish on a magnetic stir plate.

- 3 Prepare dish #3:
  - a Put the prewarmed 1.5 L glass dish on a magnetic stir plate with heating element.
  - b Put the slide-staining dish #3 into the 1.5 L glass dish.
  - c Fill the 1.5 L glass dish with pre-warmed Milli-Q ultrapure water.
  - d Fill the slide-staining dish #3 approximately three-fourths full with Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 (warmed to 37°C).
  - e Add a magnetic stir bar.
  - f Turn on the heating element and maintain temperature of Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 at 37°C. Monitor with a thermometer.
- 4 Remove one hybridization chamber from the incubator and resume rotation of the others. Record whether bubbles formed during hybridization and if all bubbles are rotating freely.
- 5 Prepare the hybridization chamber disassembly.
  - a Put the hybridization chamber assembly on a flat surface and loosen the thumbscrew, turning counter-clockwise.
  - b Slide off the clamp assembly and remove the chamber cover.
  - c With gloved fingers, remove the microarray-gasket sandwich from the chamber base by lifting one end and then grasping in the middle of the long sides. Keep the microarray slide numeric barcode facing up as you quickly transfer the sandwich to slide-staining dish #1.
  - d Without letting go of the slides, submerge the microarray-gasket sandwich into slide-staining dish #1 containing Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1.
- 6 With the sandwich completely submerged in Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1, pry the sandwich open from the barcode end only:
  - a Slip one of the blunt ends of the forceps between the slides.
  - b Gently twist the forceps to separate the slides.
  - c Let the gasket slide drop to the bottom of the staining dish.
  - d Remove the microarray slide, grasp it from the upper corners with thumb and forefinger, and quickly put into slide rack in the slide-staining dish #2 containing Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 at room temperature. Minimize exposure of the slide to air. *Touch only the barcode portion of the microarray slide or its edges!*

## 5 Microarray Processing

### Step 5. Wash microarrays

- 7 Repeat [step 4](#) through [step 6](#) for up to four additional slides in the group. A maximum of five disassembly procedures yielding five microarray slides is advised at one time in order to facilitate uniform washing.
- 8 When all slides in the group are put into the slide rack in slide-staining dish #2, stir at 350 rpm for 5 minutes. Adjust the setting to get good but not vigorous mixing.
- 9 Wash the slides in [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#):
  - a Transfer slide rack to slide-staining dish #3, which contains [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#) at 37°C:
  - a Activate the magnetic stirrer.
  - b Wash microarray slides for at least 1 minute and no more than 2 minutes. Adjust the setting to get thorough mixing without disturbing the microarray slides.
- 10 Slowly remove the slide rack trying to minimize droplets on the slides. It should take 5 to 10 seconds to remove the slide rack.
- 11 Discard used [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1](#) and [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#).
- 12 Repeat [step 1](#) through [step 11](#) for the next group of five slides using fresh [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1](#) and [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#) warmed to 37°C.
- 13 Scan slides immediately to minimize the impact of environmental oxidants on signal intensities. If necessary, store slides in orange slide boxes in a N<sub>2</sub> purge box, in the dark.

#### **Wash Procedure B (*with Stabilization and Drying Solution*)**

Cyanine reagents are susceptible to degradation by ozone. Use this wash procedure if the ozone level exceeds 10 ppb in your laboratory.

Always use fresh [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1](#) and [Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2](#) for each wash group (up to five slides).

The [Acetonitrile](#) (dish #4) and [Stabilization and Drying Solution](#) (dish #5) below may be reused for washing up to 4 batches of 5 slides (total 20 slides) in one experiment. Do not pour the [Stabilization and Drying Solution](#) back in the bottle.

**WARNING**

The **Stabilization and Drying Solution** must be set-up in a fume hood. Put the **Wash Buffer 1** and **Wash Buffer 2** set-up areas close to, or preferably in, the same fume hood. Use gloves and eye/face protection in every step of the washing procedure.

Table 42 lists the wash conditions for the Wash Procedure B with **Stabilization and Drying Solution**.

**Table 42** Wash conditions

	Dish	Wash Buffer	Temperature	Time
Disassembly	#1	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1	Room temperature	
1st wash	#2	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1	Room temperature	5 minutes
2nd wash	#3	Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2	37°C	1 minute
Acetonitrile wash	#4	Acetonitrile	Room temperature	10 seconds
3rd wash	#5	Stabilization and Drying Solution	Room temperature	30 seconds

- 1 In the fume hood, fill slide-staining dish #4 approximately three-fourths full with **Acetonitrile**. Add a magnetic stir bar and put this dish on a magnetic stir plate.
- 2 In the fume hood, fill slide-staining dish #5 approximately three-fourths full with **Stabilization and Drying Solution**. Add a magnetic stir bar and put this dish on a magnetic stir plate.
- 3 Do step 1 through step 9 in “Wash Procedure A (without Stabilization and Drying Solution)” on page 74.
- 4 Remove the slide rack from **Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2** and tilt the rack slightly to minimize wash buffer carry-over. Quickly transfer the slide rack to slide-staining dish #4 containing **Acetonitrile**, and stir at 350 rpm for 10 seconds.
- 5 Transfer slide rack to slide-staining dish #5 filled with **Stabilization and Drying Solution**, and stir at 350 rpm for 30 seconds.

## 5 Microarray Processing

### Step 5. Wash microarrays

- 6 Slowly remove the slide rack trying to minimize droplets on the slides. It should take 5 to 10 seconds to remove the slide rack.
- 7 Discard used Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 and Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2.

#### NOTE

The Acetonitrile and the Stabilization and Drying Solution may be reused for washing of up to four batches of five slides (that is, total 20 microarray slides) in one experiment. Pour the Stabilization and Drying Solution to a different marked bottle, and protect from light with other flammables. After each use, rinse the slide rack and the slide-staining dish that were in contact with the Stabilization and Drying Solution with Acetonitrile followed by a rinse in Milli-Q ultrapure water.

---

- 8 Repeat step 1 through step 7 for the next group of five slides using fresh Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1 and Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2 prewarmed to 37°C.
- 9 Dispose of Acetonitrile and Stabilization and Drying Solution as flammable solvents.

## Step 6. Put slides in a slide holder

Scan slides immediately to minimize impact of environmental oxidants on signal intensities. If necessary, store slides in the original slide boxes in a N<sub>2</sub> purge box, in the dark.

### For SureScan microarray scanner

- 1 Carefully place the end of the slide without the barcode label onto the slide ledge.
- 2 Gently lower the microarray slide into the slide holder. Make sure that the active microarray surface (with “Agilent”-labeled barcode) faces up, toward the slide cover.
- 3 Close the plastic slide cover, pushing on the tab end until you hear it click.

For more detailed instruction, refer to the *Agilent G4900DA SureScan Microarray Scanner System User Guide*.




**Figure 4** Slide in slide holder for SureScan microarray scanner

### For Agilent Scanner B or C

- In environments in which the ozone level exceeds 5 ppb, immediately put the slides with active microarray surface (“Agilent”-labeled barcode) facing up in a slide holder. Make sure that the slide is not caught up on any corner. Put an ozone-barrier slide cover on top of the array as shown in [Figure 5](#). Refer to the *Agilent Ozone-Barrier Slide Cover User Guide* (p/n G2505-90550), included with the slide cover, for more information.

## 5 Microarray Processing

### Step 6. Put slides in a slide holder

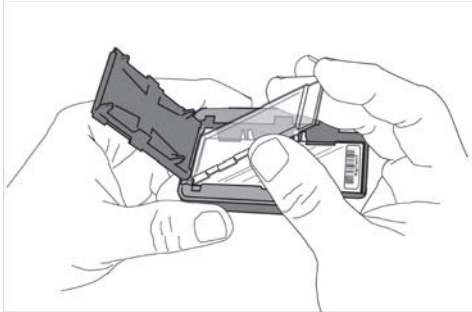

**Figure 5** Inserting the ozone-barrier slide cover

- In environments in which the ozone level is below 5 ppb, put the slides with Agilent barcode facing up in a slide holder.



# Microarray Scanning and Analysis

## Step 1. Scan the microarray slides

A SureScan or Agilent C microarray scanner is required for G3 microarrays.

Agilent provides support for Agilent microarrays scanned on select non-Agilent scanners. Please see “Feature Extraction Compatibility Matrix for Non Agilent scanners” for scanner compatibility and settings ([http://www.chem.agilent.com/Library/usermanuals/Public/G1662-90043\\_ScannerCompatibilityMatrix.pdf](http://www.chem.agilent.com/Library/usermanuals/Public/G1662-90043_ScannerCompatibilityMatrix.pdf)).

*However, Agilent can guarantee the quality of data only if the data comes from Agilent microarrays scanned on Agilent scanners.*

### Agilent SureScan Microarray Scanner

- 1 Put assembled slide holders into the scanner cassette.
- 2 Select **Protocol AgilentG3\_CGH** for G3 microarrays. Select **Protocol AgilentHD\_CGH** for HD microarrays.
- 3 Verify that the Scanner status in the main window says Scanner Ready.
- 4 Click **Start Scan**.

### Agilent C Scanner Settings

- 1 Put assembled slide holders with or without the ozone-barrier slide cover into scanner carousel.
- 2 Select Start Slot *m* End Slot *n* where the letter *m* represents the Start slot where the first slide is located and the letter *n* represents the End slot where the last slide is located.
- 3 Select **Profile AgilentG3\_CGH** for G3 microarrays. Select **Profile AgilentHD\_CGH** for HD microarrays.
- 4 Verify scan settings. See [Table 43](#).

## 5 Microarray Processing

### Step 1. Scan the microarray slides

**Table 43** C Scanner Scan Settings

	For HD Microarray Formats	For G3 Microarray Formats
<b>Dye channel</b>	R+G ( <i>red and green</i> )	R+G ( <i>red and green</i> )
<b>Scan region</b>	Agilent HD (61 x 21.6 mm)	Agilent HD (61 x 21.6 mm)
<b>Scan resolution</b>	5 $\mu\text{m}$	3 $\mu\text{m}$
<b>Tiff file dynamic range</b>	16 bit	16 bit
<b>Red PMT gain</b>	100%	100%
<b>Green PMT gain</b>	100%	100%
<b>XDR</b>	<No XDR>	<No XDR>

**5** Check that **Output Path Browse** is set for desired location.

**6** Verify that the Scanner status in the main window says Scanner Ready.

**7** Click **Scan Slot *m-n*** on the Scan Control main window where the letter *m* represents the Start slot where the first slide is located and the letter *n* represents the End slot where the last slide is located.

### Agilent B Scanner Settings

Agilent Scanner Control software v7.0.03 is recommended for 5  $\mu\text{m}$  scans of HD format microarrays.

**1** Put assembled slide holders, with or without the ozone-barrier slide cover, into scanner carousel.

**2** Verify Default Scan Settings (click **Settings > Modify Default Settings**).

**Table 44** B Scanner Scan Settings

	For HD Microarray Formats
Scan region	Scan Area (61 x 21.6 mm)
Scan resolution ( $\mu\text{m}$ )	5
eXtended Dynamic range	(cleared)
Dye channel	Red&Green
Red PMT	100%
Green PMT	100%

- 3 Select settings for the automatic file naming.
  - **Prefix1** is set to **Instrument Serial Number**.
  - **Prefix2** is set to **Array Barcode**.
- 4 Verify that the Scanner status in the main window says **Scanner Ready**.
- 5 Click **Scan Slot *m-n*** on the Scan Control main window where the letter *m* represents the Start slot where the first slide is located and the letter *n* represents the End slot where the last slide is located.

## Step 2. Analyze microarray image

- After scanning is completed, extract features and analyze.

Feature extraction is the process by which data is extracted from the scanned microarray image (.tif) and translated into log ratios, allowing researchers to identify aberrations in their samples.

Agilent provides Feature Extraction software as a standalone program and as an integral part of CytoGenomics software (Windows version only).

- Use the Windows version of Agilent CytoGenomics for automated and streamlined analysis of human samples. During the extraction and analysis process, Agilent CytoGenomics generates feature extraction files, QC and aberration reports.
- To use Agilent CytoGenomics on a Mac computer, first use Feature Extraction on a computer that is running Windows to extract features. Feature Extraction does not run on Mac computers.
- For non-human samples, use Feature Extraction (available for Windows only) to extract features, and then use Agilent Genomic Workbench to run an analysis workflow on the extracted features.

### Microarray QC Metrics for high DNA quality samples

These metrics are only appropriate for high-quality DNA samples analyzed with Agilent CGH microarrays by following the standard operational procedures provided in this user guide. These metrics are reported in the Feature Extraction QC report generated by Feature Extraction (standalone or as included in the Agilent CytoGenomics software). They can be used to assess the relative data quality from a set of microarrays in an experiment. In some cases, they can indicate potential processing errors that have occurred or

## 5 Microarray Processing

### Step 2. Analyze microarray image

suggest that the data from particular microarrays might be compromised. Many factors can influence the range of these metrics, including the microarray format (1-pack, 2-pack, 4-pack or 8-pack), biological sample source, quality of starting gDNA, experimental processing, scanner sensitivity, and image processing. The value guidelines presented below represent the thresholds that Agilent has observed when analyzing samples using this protocol.

To achieve a high SNP call rate and accuracy when processing SurePrint G3 CGH+SNP microarrays, make sure the DLRSD is <0.2.

**Table 45** QC metric thresholds for Enzymatic labeling

Metric	Excellent	Good	Evaluate
BGNoise	< 10	10 to 20	> 20
Signal Intensity	> 150	50 to 150	< 50
Signal to Noise	> 100	30 to 100	< 30
Reproducibility	< 0.05	0.05 to 0.2	> 0.2
DLRSD	< 0.2	0.2 to 0.3	> 0.3


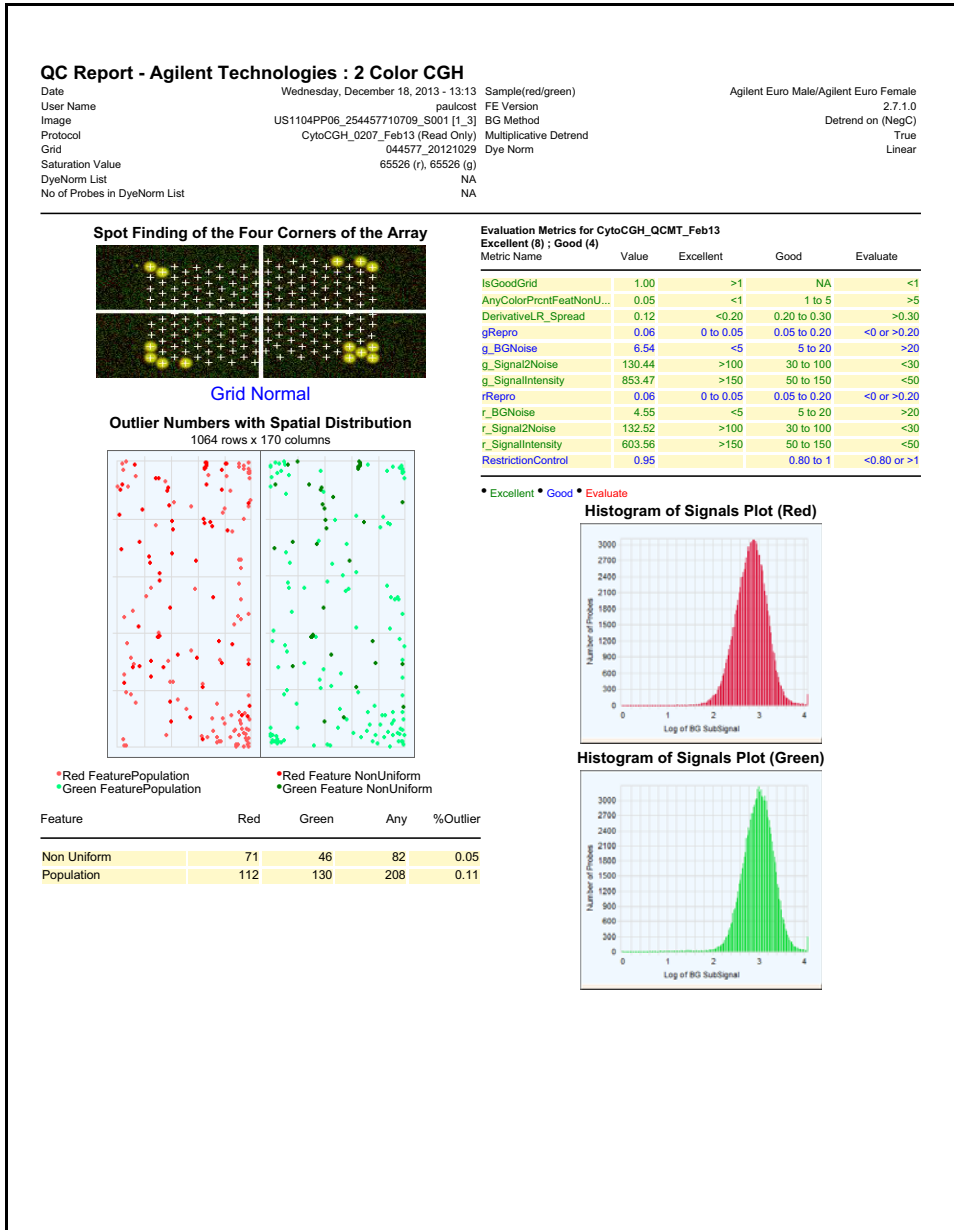


Figure 6 Feature Extraction QC Report, page 1

5 **Microarray Processing**  
Step 2. Analyze microarray image

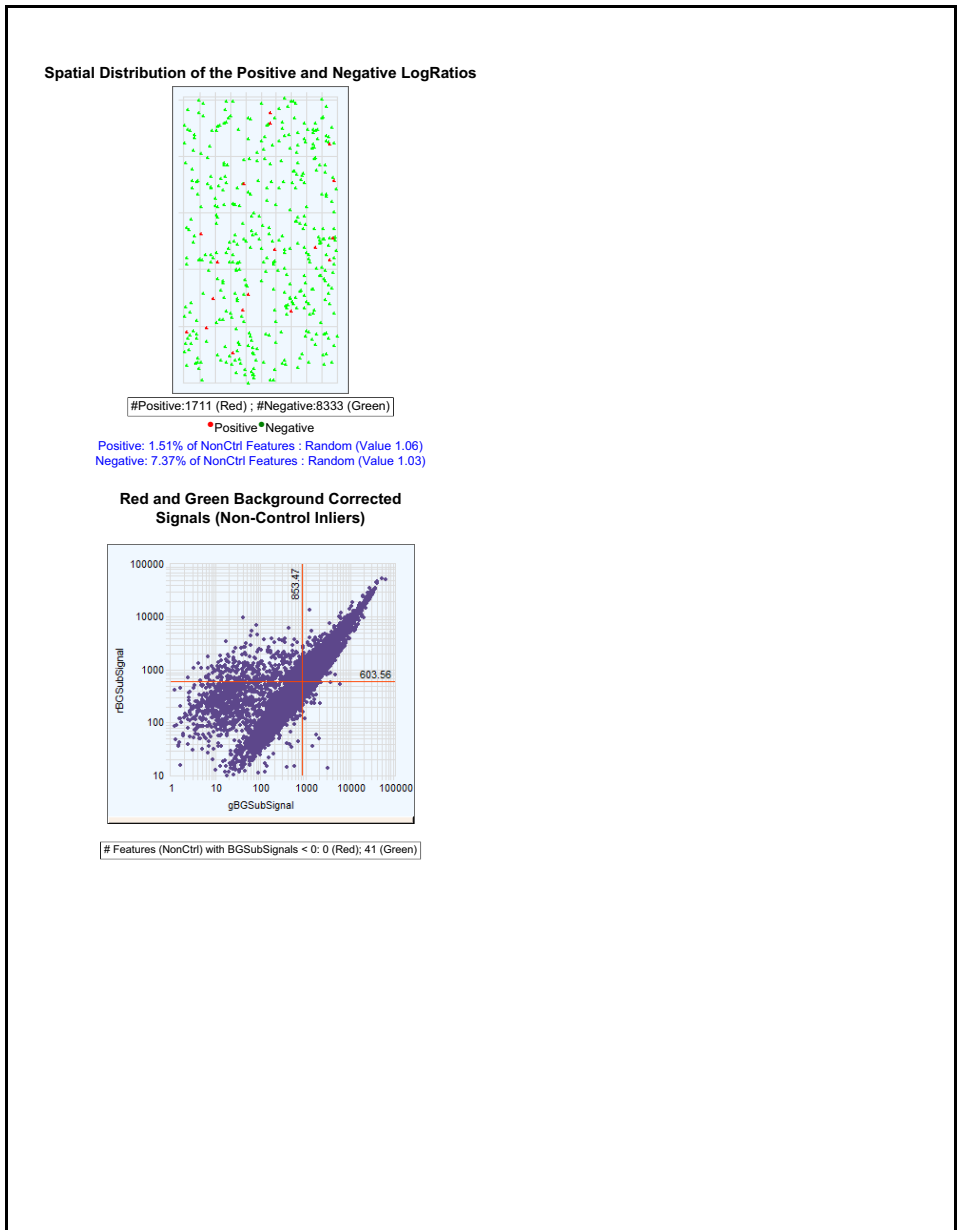

**Figure 7** Feature Extraction QC Report, page 2

## Step 3. Download Agilent Reference Genotype File

To analyze your data when you have used the [Human Reference DNA \(Male and Female\)](#) and CGH+SNP microarrays with Agilent CytoGenomics 2.0 or Genomic Workbench 6.5 or higher, you need to get the Agilent Reference Genotype File (Male and Female) from Agilent.


The Reference Genotype File is included with Agilent CytoGenomics 2.7.

- 1 Go to <http://www.genomics.agilent.com/article.jsp?pageId=3299>.
- 2 Click the **Download** link for **Agilent Reference Genotype Files (Male and Female)**.
- 3 Click **Save** to save the files.

To load the Agilent Reference Genotype Files (Male and Female), refer to the user guide for Agilent CytoGenomics or Agilent Genomic Workbench.

**This page intentionally left blank.**



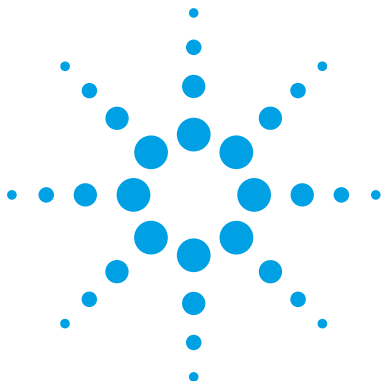

## 6 Troubleshooting

- If you have a low OD<sub>260</sub>/<sub>230</sub> or OD<sub>260</sub>/<sub>280</sub> value 90
- If you have poor sample quality due to residual RNA 90
- If you get poor sample quality due to degradation 91
- If the estimated concentration is too high or low 92
- If you have low specific activity or degree of labeling not due to poor sample quality 93
- If you have low yield not due to poor sample quality 93
- If you have post-labeling signal loss 94
- If you have high BGNoise values 95
- If you have poor reproducibility 95

This chapter contains potential causes for above-threshold DLRSD (Derivative Log Ratio Standard Deviation). A poor DLRSD score reflects high probe-to-probe log ratio noise.



## If you have a low OD260/230 or OD260/280 value

A low OD260/230 value can indicate contaminants, such as residual salt or organic solvents (which would inhibit enzyme). A low OD260/280 value indicates residual protein. Either condition can result in low specific activity (pmol dye/ $\mu$ g DNA) or Degree of Labeling. See “To determine yield, and degree of labeling or specific activity” on page 61.

- ✓ Repurify the DNA using the Qiagen DNeasy protocol. See “DNA Isolation” on page 27. This procedure includes a proteinase K treatment.
- ✓ If you must do a phenol/chloroform DNA extraction, do not get too close to the interface.  
  
Phenol has an absorbance maximum of 270–275 nm, which is close to that of DNA. Phenol contamination mimics both higher purity and higher yields, because of an upward shift in the OD260 value.
- ✓ Make sure to calibrate the spectrophotometer with the appropriate buffer.

## If you have poor sample quality due to residual RNA

The input amount of DNA for the experimental sample must be the same as for the reference sample. RNA absorbs at the same wavelength as DNA. Therefore, RNA-contaminated sample can result in a DNA overestimation.

- ✓ Repurify the DNA using the Qiagen DNeasy protocol. See “DNA Isolation” on page 27. This procedure includes a RNase A treatment.

## If you get poor sample quality due to degradation

For non-FFPE samples: On a 1 to 1.5% agarose gel, intact gDNA should appear as a compact, high-molecular weight band with no lower molecular weight smears. Degraded DNA results in biased labeling.

- ✓ Check DNA on a 1 to 1.5% agarose gel. If DNA that was isolated from cells, blood or frozen tissue is degraded, then repurify the DNA using the Qiagen DNeasy protocol. See “DNA Isolation” on page 27.
- ✓ If you replace the restriction digestion step by a longer incubation at 98°C, make sure that the DNA is not over-fragmented prior to labeling. Possible causes are incorrect temperature or length of incubation at 98°C, or evaporation (use a thermal cycler with heated lid). Make sure most of the heat fragmented products are between 1000 and 3000 bases in length.
- ✓ For processing FFPE samples, refer to the *Agilent Oligonucleotide Array-Based CGH for Genomic DNA Analysis (ULS Labeling for Blood, Cells, Tissues or FFPE) Protocol* (p/n G4410-90020). FFPE samples are not supported when you process SurePrint G3 CGH+SNP microarrays.

## If the estimated concentration is too high or low

The input amount of DNA for the experimental sample must be the same as for the reference sample. Precipitated DNA or DNA that is at a very high concentration cannot be quantitated accurately.

Contaminants such as organic solvents and RNA also absorb at 260 nm, which results in an inaccurate DNA quantitation.

- ✓ Make sure that the gDNA is completely in solution by pipetting up and down. If needed, incubate at 37°C for 30 minutes. If the gDNA concentration is > 350 ng/μL, dilute 1:2 in [Buffer AE](#) or [1×TE \(pH 8.0\)](#). Quantitate again to make sure quantitation is accurate.
- ✓ Different DNA isolation methods can create different quantitation artifacts, the risk of assay noise is higher when the experimental and reference DNA samples are isolated from different sources. If you used a spectrophotometer (such as the Nanodrop) for the initial measurement, also use a double-stranded DNA-based fluorometer (such as the Qubit) to verify.
- ✓ If needed, repurify the DNA using the Qiagen DNeasy protocol. See “[DNA Isolation](#)” on page 27.

If you have low specific activity or degree of labeling not due to poor sample quality

## If you have low specific activity or degree of labeling not due to poor sample quality

Low specific activity or degree of labeling can result from sub-optimal labeling conditions such as Cyanine dUTP with too many freeze thaws, enzyme degradation due to being left warm for too long, wrong temperatures or times, volume mistakes, or too much exposure to light or air.

- ✓ Store Cyanine dUTP at -20°C. Keep enzymes on ice and return to -20°C as quickly as possible.
- ✓ Double check incubation times and temperatures (use a calibrated thermometer), and use a thermal cycler with heated lid.
- ✓ Evaporation can be a problem when you process samples at high temperatures. Make sure that sample tubes are well closed or use a plate [Heat Sealer](#) to avoid evaporation.
- ✓ Make sure that the pipettors are not out of calibration.
- ✓ Make sure that the gDNA, reagents, and master mixes are well mixed. Tap the tube with your finger or use a pipette to move the entire volume up and down. Then spin in a microcentrifuge for 5 to 10 seconds to drive the contents off the walls and lid. Do not mix the stock solutions and reactions that contain gDNA or enzymes on a vortex mixer.

## If you have low yield not due to poor sample quality

Possible sample loss during clean-up after labeling.

- ✓ See “[Step 2. Purification of Labeled gDNA](#)” on [page 56](#) to remove unreacted dye. Many other columns result in the loss of shorter fragments.

## If you have post-labeling signal loss

Signal loss can be due to wash or hybridization conditions that are too stringent, or degradation of the Cyanine 5 signal.

Cyanine 5 signal degradation can be caused by ozone or NO<sub>x</sub> compounds coming from pollution and/or compressors and centrifuges. Cyanine 5 signal degradation can result in less red signal around the edges of the features, a visible gradient of significant Cy5/Cy3 positive ratios and more significant Cy5/Cy3 negative ratios – especially on the left side of the slide and on slides scanned later in a batch.

- ✓ Check that the oven temperature is 67°C. If needed, recalibrate the hybridization oven. Follow the steps in *Agilent G2545A Hybridization Calibration Procedure* (p/n G2545-90002).
- ✓ Check that the temperature of Wash 2 is 37°C.
- ✓ Check that Wash 2 was not accidentally used instead of Wash 1.
- ✓ Wash and scan slides in an ozone controlled environment (<5 ppb), such as an ozone tent.
- ✓ Use small batches that can be washed and scanned in about 40 minutes to minimize exposure to air.
- ✓ For Agilent Scanner C or B, use the Agilent Ozone-Barrier Slide Cover (p/n G2505-60550). The SureScan scanner has built-in ozone protection.
- ✓ Use the [Stabilization and Drying Solution](#) as described in “[Wash Procedure B \(with Stabilization and Drying Solution\)](#)” on page 76.

## If you have high BGNoise values

High BGNoise can cause lower signal-to-noise values (see [Table 45](#) for thresholds) and higher DLRSD values. BGNoise is defined as the standard deviation of the signals on the negative controls. If the BGNoise is high, examine the microarray image for visible non-uniformities. High BGNoise is often introduced during hybridization steps or washes.

- ✓ Make sure that the oven is calibrated. Follow the steps in *Agilent G2545A Hybridization Calibration Procedure* (p/n G2545-90002).

Sample hybridization at incorrect temperatures affects the stringency of the hybridization.

- ✓ Make sure that wash dishes, racks and stir bars are clean. Do not use tap water or detergents to clean wash equipment. If needed, rinse wash equipment with acetonitrile followed by rinses with MilliQ water.

- ✓ If needed, wash the slides with acetonitrile:

- 1 In the fume hood, fill a slide-staining dish approximately three-fourths full with acetonitrile.
- 2 Add a magnetic stir bar and put this dish on a magnetic stir plate.
- 3 Put the slides in a slide rack and transfer the slide rack to the slide-staining dish containing acetonitrile, and stir at 350 rpm for 1 minute.
- 4 Slowly remove the slide rack and scan the slides immediately.


## If you have poor reproducibility

Poor reproducibility (see [Table 45](#) for thresholds), defined as high CVs of signals of replicated probes may indicate that the hybridization volume was too low or that the oven stopped rotating during the hybridization. Only very high scores on this metric will affect the DLRSD.

- ✓ When setting up the gasket-slide hybridization sandwich dispense the hybridization sample mixture slowly in a “drag and dispense” manner to prevent spills.
- ✓ Check that the oven is rotating.

**This page intentionally left blank.**



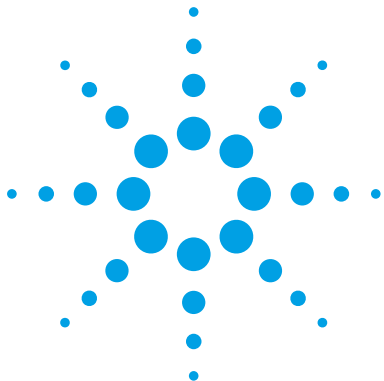

## 7 Reference

Reagent Kit Components	98
Microarray Handling Tips	101
Agilent Microarray Layout and Orientation	102
Array/Sample tracking on microarray slides	105

This chapter contains reference information that pertains to this protocol.



## Reagent Kit Components

The contents of the reagent kits used in this protocol are listed here.

**Table 46** DNeasy Blood & Tissue Kit

Component
DNeasy Mini Spin Column
2 mL Collection Tube
Buffer ATL
Buffer AL
Buffer AW1
Buffer AW2
Buffer AE
Proteinase K

**Table 47** Qubit dsDNA BR Assay Kit

Component
Qubit dsDNA BR reagent
Qubit dsDNA BR buffer
Qubit dsDNA BR standard #1
Qubit dsDNA BR standard #2

**Table 48** SureTag Complete DNA Labeling Kit and SureTag DNA Labeling Kit

Component
Human Reference DNA (Male and Female)*
10× Restriction Enzyme Buffer
BSA
Alu I
Rsa I
Purification Column
Nuclease-Free Water
Exo (-) Klenow
5× Reaction Buffer
Cyanine 5-dUTP
Cyanine 3-dUTP
10× dNTPs
Random Primer

\* Included in the SureTag Complete DNA Labeling Kit only.

**Table 49** GenomePlex Complete Whole Genome Amplification Kit

Component
1× Library Preparation Buffer
10× Fragmentation Buffer
Control Human Genomic DNA
Library Preparation Enzyme
10× Amplification Master Mix
Library Stabilization Solution
WGA DNA Polymerase
Nuclease-Free Water

**7 Reference**  
**Reagent Kit Components**

**Table 50** GenElute PCR Clean-Up Kit

Component
Column Preparation Solution
Binding Solution
Wash Solution Concentrate
Elution Solution
GenElute plasmid mini spin column
2 mL Collection Tube

**Table 51** Oligo aCGH/ChIP-on-chip Hybridization Kit

Component
2× HI-RPM Hybridization Buffer
10× aCGH Blocking Agent

**Table 52** Oligo aCGH/ChIP-on-chip Wash Buffer Kit

Component
Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 1
Agilent Oligo aCGH/ChIP-on-Chip Wash Buffer 2

## Microarray Handling Tips

Each microarray is printed on the side of the glass slide containing the “Agilent”-labeled barcode. This side is called the “active” side. The numeric barcode is on the inactive side of the slide.

### CAUTION

You must familiarize yourself with the assembly and disassembly instructions for use with the Agilent Microarray Hybridization Chamber (G2534A) and gasket slides. Practice slide kits are available.

---


In this “processing and hybridization” procedure, the hybridization mixture is applied directly to the gasket slide, and not to the active side of the oligo microarray. Instead, the active side of the oligo microarray is placed on top of the gasket slide to form a “sandwich slide” pair.

To avoid damaging the microarray, always handle glass slides carefully by their edges. Wear powder-free gloves. Never touch the surfaces of the slides. If you do, you may cause irreparable damage to the microarray.

Never allow the microarray surface to dry out during the hybridization process and washing steps.

## Agilent Microarray Layout and Orientation

### Agilent oligo microarray (1 microarray/slide format) as imaged on the Agilent microarray scanner

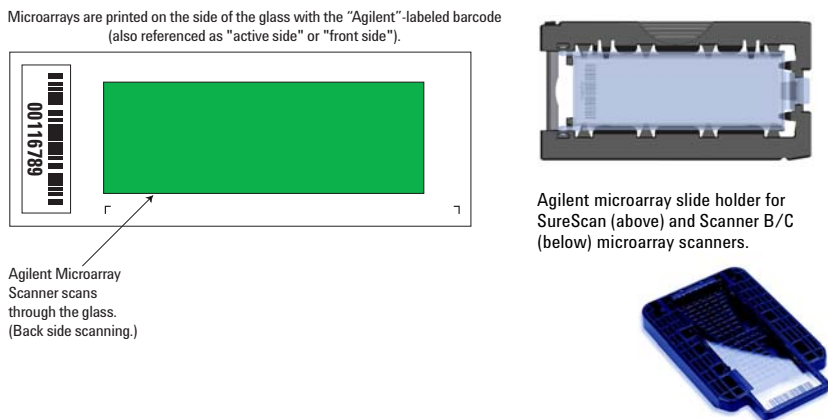

**Figure 8** Agilent microarray slide and slide holder

Agilent oligo microarrays formats and the resulting "microarray design files" are based on how the Agilent microarray scanner images 1-inch x 3-inch glass slides. Agilent designed its microarray scanner to scan through the glass slide (back side scanning). The glass slide is securely placed in an Agilent microarray slide holder with the "Agilent" labeled barcode facing the opening of the slide holder (on SureScan Microarray Scanner) or facing the inside of the slide holder (Scanner C or Scanner B). In this orientation, the "active side" containing the microarrays is protected from potential damage by fingerprints and other elements. Once securely placed, the numeric barcode, non-active side of the slide, is visible from the outside of the slide holder.

Figure 8 depicts how the Agilent microarray scanner reads the microarrays and how this relates to the "microarray design files" that Agilent generates during the manufacturing process of its *in situ*-synthesized oligonucleotide microarrays. Thus, if you have a scanner that reads microarrays from the "front side" of the glass slide, the collection of microarray data points will be different in relation to the "microarray design files". Therefore, please take a

moment to become familiar with the microarray layouts for each of the Agilent oligo microarrays and the layout information as it pertains to scanning using a “front side” scanner.

### **Non-Agilent Front Side Microarray Scanners**


When scanning Agilent oligo microarray slides, the user must determine:

- If the scanner images the microarrays by reading them on the “front side” of the glass slide (“Agilent”-labeled barcode side of the slide) and
- If the microarray image produced by the non-Agilent scanner is oriented in a “portrait” or “landscape” mode, and “Agilent”-labeled barcode is on the left-side, right-side, up or down, as viewed as an image in the imaging software (see [Figure 9](#)).

This changes the feature numbering and location as it relates to the “microarray design files”.

## 7 Reference

### Agilent Microarray Layout and Orientation

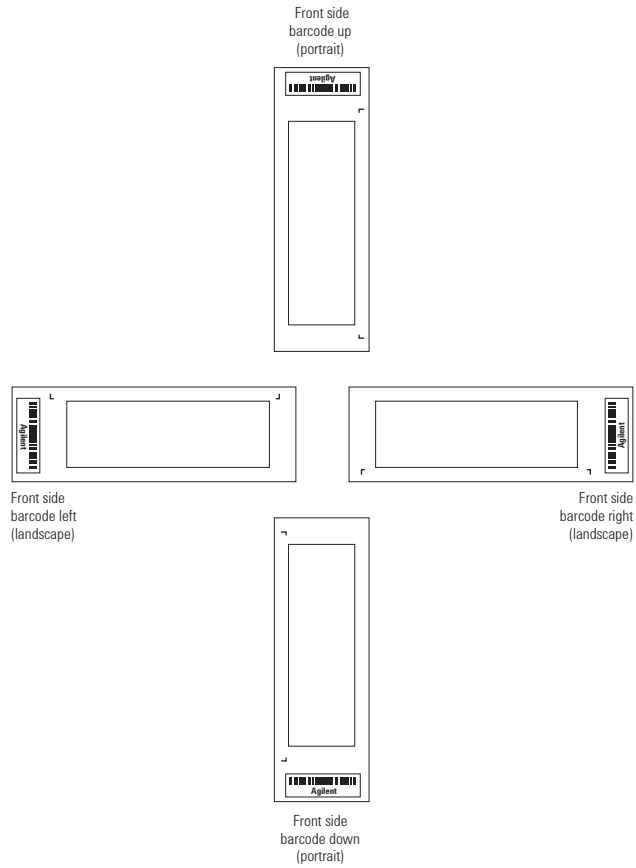

**Figure 9** Microarray slide orientation



## Array/Sample tracking on microarray slides

Use the forms below to make notes to track your samples on microarray slides.

Position the gasket slide in the SureHyb chamber base with the label to the left and load the samples: top row, left to right, then lower row, left to right. The array suffix assignments from Feature Extraction will then occur in the order shown.

### Arrays

Array 1\_1

Array 1\_2

B A R C O D E	Sample:	Sample:

Barcode Number \_\_\_\_\_

**Figure 10** 2-pack microarray slides

**7 Reference**

Array/Sample tracking on microarray slides

**Arrays**

	Array 1_1	Array 1_2	Array 1_3	Array 1_4
<b>B A R C O D E</b>	Sample:	Sample:	Sample:	Sample:
<b>Barcode Number</b> _____				

**Figure 11** 4-pack microarray slides

## Arrays

		Array 1_1	Array 1_2	Array 1_3	Array 1_4
B A R C O D E	<b>Sample:</b>				
	<b>Sample:</b>				
		Array 2_1	Array 2_2	Array 2_3	Array 2_4

**Barcode Number** \_\_\_\_\_

**Figure 12** 8-pack microarray slide

[www.agilent.com](http://www.agilent.com)

## In This Book

This guide contains information to run the Oligonucleotide Array-Based CGH for Genomic DNA Analysis – Enzymatic Labeling for Blood, Cells, or Tissues (with a High Throughput option) protocol.

© Agilent Technologies, Inc. 2009-2015

Version 7.4, August 2015



G4410-90010  
Revision B3



**Agilent Technologies**